



US007497863B2

(12) **United States Patent**  
**Solar et al.**

(10) **Patent No.:** **US 7,497,863 B2**  
(45) **Date of Patent:** **Mar. 3, 2009**

(54) **INSTRUMENT GUIDING STAGE APPARATUS AND METHOD FOR USING SAME**

3,115,140 A 12/1963 Volkman  
3,135,263 A 6/1964 Connelley, Jr.  
3,223,087 A 12/1965 Vladyka et al.  
3,262,452 A 7/1966 Hardy et al.

(75) Inventors: **Matthew S. Solar**, Indialantic, FL (US);  
**Thomas I. Miller**, Palm Bay, FL (US);  
**James G. Skakoon**, St. Paul, MN (US)

(Continued)

(73) Assignee: **Medtronic, Inc.**, Minneapolis, MN (US)

FOREIGN PATENT DOCUMENTS

DE 3108766 9/1982

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 331 days.

(Continued)

(21) Appl. No.: **11/005,607**

OTHER PUBLICATIONS

“Cross-Hairs Kit”, Elekta Instruction for Use Brochure, pp. 1-5.

(22) Filed: **Dec. 4, 2004**

(Continued)

(65) **Prior Publication Data**

US 2006/0122628 A1 Jun. 8, 2006

*Primary Examiner*—Darwin P Erez  
*Assistant Examiner*—Gregory A Anderson  
(74) *Attorney, Agent, or Firm*—Harness, Dickey & Pierce, P.L.C.

(51) **Int. Cl.**  
**A61B 19/00** (2006.01)

(52) **U.S. Cl.** ..... **606/130**

(58) **Field of Classification Search** ..... 606/219,  
606/129, 130; 359/368; 74/640, 411, 464  
See application file for complete search history.

(57) **ABSTRACT**


This documents describes among other things a normalizing stage apparatus, tools and methods. One example includes a base that defines a trajectory. A first stage is moveably coupled to the base and the first stage moves along the trajectory. A second stage is moveably coupled to the first stage and moves an instrument coupled thereto with respect to the base and the first stage. Before movement of the instrument, the first and second stages are in first positions desired (e.g. predetermined) distances from a target area in the body. Another example includes the first stage and a guide tube stop coupled with the first stage. A guide tube is coupled with the guide tube stop and extends through a guide tube stop lumen. The guide tubes outer perimeter is dimensioned and configured to snugly couple with the surface defining the guide tube stop lumen.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,129,333 A 2/1915 Clarke  
1,664,210 A 3/1928 Hall  
2,119,649 A 6/1938 Roosen  
2,135,160 A 11/1938 Beekhuis  
2,686,890 A \* 8/1954 Davis ..... 74/110  
3,016,899 A 1/1962 Stenvall  
3,017,887 A 1/1962 Heyer  
3,055,370 A 9/1962 McKinney et al.  
3,055,371 A 9/1962 Kulick et al.

**32 Claims, 35 Drawing Sheets**

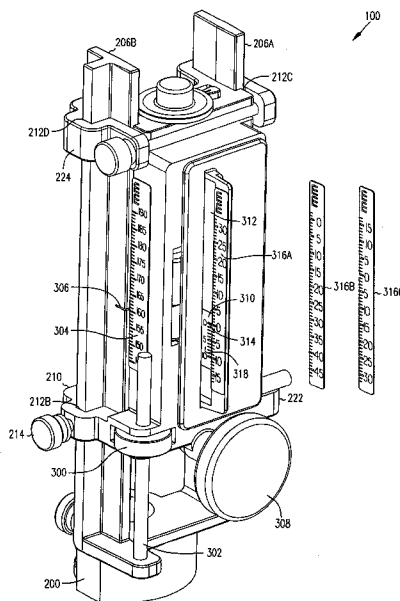

U.S. PATENT DOCUMENTS							
3,273,559	A	9/1966	Evans	5,054,497	A	10/1991	Kapp et al.
3,282,152	A	11/1966	Myer	5,057,084	A	10/1991	Ensminger et al.
3,402,710	A	9/1968	Paleschuck	5,057,106	A	10/1991	Kasevich et al.
3,444,861	A	5/1969	Schulte	5,078,140	A	1/1992	Kwoh
3,457,922	A	7/1969	Ray	5,078,142	A	1/1992	Siczek et al.
3,460,537	A	8/1969	Zeis	5,080,662	A	1/1992	Paul
3,508,552	A	4/1970	Hainault	5,087,256	A	2/1992	Taylor et al.
3,672,352	A	6/1972	Summers	5,099,846	A	3/1992	Hardy
3,760,811	A	9/1973	Andrew et al.	5,102,402	A	4/1992	Dror et al.
3,893,449	A	7/1975	Lee et al.	5,116,344	A	5/1992	Sundqvist et al.
3,981,079	A	9/1976	Lenczycki	5,116,345	A	5/1992	Jewell et al.
4,013,080	A	* 3/1977	Froning ..... 604/165.01	5,120,322	A	6/1992	Davis et al.
4,040,427	A	8/1977	Winnie	5,125,888	A	6/1992	Howard et al.
4,230,117	A	10/1980	Anichkov et al.	5,142,930	A	9/1992	Allen et al.
4,265,252	A	5/1981	Chubuck et al.	5,143,086	A	9/1992	Duret et al.
4,312,337	A	1/1982	Donohue	5,154,179	A	10/1992	Ratner
4,318,401	A	* 3/1982	Zimmerman ..... 604/28	5,154,723	A	10/1992	Kubota et al.
4,328,813	A	5/1982	Ray	5,163,430	A	11/1992	Carol
4,341,220	A	7/1982	Perry	5,166,875	A	11/1992	Machida et al.
4,345,606	A	8/1982	Littleford	5,171,217	A	12/1992	March et al.
4,350,159	A	9/1982	Gouda	5,174,297	A	12/1992	Daikuzono et al.
4,355,645	A	10/1982	Mitani et al.	5,186,174	A	2/1993	Schlondorff et al.
4,386,602	A	6/1983	Sheldon et al.	5,201,742	A	4/1993	Hasson
4,418,894	A	12/1983	Mailliet et al.	5,207,223	A	5/1993	Adler
4,448,195	A	5/1984	LeVeon et al.	5,207,688	A	5/1993	Carol
4,463,758	A	8/1984	Patil et al.	5,211,165	A	5/1993	Dumoulin et al.
4,475,550	A	10/1984	Bremer et al.	5,221,264	A	6/1993	Wilk et al.
4,483,344	A	11/1984	Atkov et al.	5,222,499	A	6/1993	Allen et al.
4,571,750	A	2/1986	Barry	5,230,338	A	7/1993	Allen et al.
4,572,198	A	2/1986	Codrington	5,230,623	A	7/1993	Guthrie et al.
4,579,120	A	4/1986	MacGregor	5,246,448	A	9/1993	Chang
4,592,352	A	6/1986	Patil	5,257,998	A	11/1993	Ota et al.
4,598,708	A	7/1986	Beranek	5,263,939	A	11/1993	Wortrich
4,608,977	A	9/1986	Brown	5,263,956	A	11/1993	Nobles
4,617,925	A	10/1986	Laitinen et al.	5,267,970	A	12/1993	Chin et al.
4,618,978	A	10/1986	Cosman	5,269,305	A	12/1993	Corol
4,629,451	A	12/1986	Winters et al.	5,279,309	A	1/1994	Taylor et al.
4,638,798	A	1/1987	Shelden et al.	5,279,575	A	1/1994	Sugarbaker
4,660,563	A	4/1987	Lees	5,280,427	A	1/1994	Magnusson et al.
4,665,928	A	5/1987	Linial et al.	5,290,266	A	3/1994	Rohling et al.
4,699,616	A	10/1987	Nowak et al.	5,291,890	A	3/1994	Cline et al.
4,705,436	A	11/1987	Robertson et al.	5,300,080	A	4/1994	Clayman et al.
4,706,665	A	11/1987	Gouda	5,305,203	A	4/1994	Raab et al.
4,733,661	A	3/1988	Palestrant	5,306,272	A	4/1994	Cohen et al.
4,755,642	A	7/1988	Parks	5,309,913	A	5/1994	Kormos et al.
4,791,934	A	12/1988	Brunnett	5,330,485	A	7/1994	Clayman et al.
4,793,355	A	12/1988	Crum et al.	5,354,283	A	10/1994	Bark et al.
4,805,615	A	2/1989	Carol	5,361,763	A	11/1994	Kao et al.
4,805,634	A	2/1989	Ullrich et al.	5,366,446	A	11/1994	Tal et al.
4,807,620	A	2/1989	Strul et al.	5,375,588	A	12/1994	Yoon
4,809,694	A	3/1989	Ferrara	5,375,596	A	12/1994	Twiss et al.
4,824,436	A	4/1989	Wolinsky	5,380,302	A	1/1995	Orth
4,826,487	A	5/1989	Winter	5,383,454	A	1/1995	Bucholz
4,869,247	A	9/1989	Howard, III et al.	5,387,220	A	2/1995	Pisharodi
4,883,053	A	11/1989	Simon	5,394,457	A	2/1995	Leibinger et al.
4,896,673	A	1/1990	Rose et al.	5,405,330	A	4/1995	Zunitch et al.
4,902,129	A	2/1990	Siegmund et al.	5,423,848	A	6/1995	Washizuka et al.
4,922,924	A	5/1990	Gambale et al.	5,445,166	A	8/1995	Taylor
4,955,891	A	9/1990	Carol	5,452,720	A	9/1995	Smith et al.
4,957,481	A	9/1990	Gatenby	5,464,446	A	11/1995	Dreessen et al.
4,986,280	A	1/1991	Marcus et al.	5,470,307	A	11/1995	Lindall
4,986,281	A	1/1991	Preves et al.	5,474,564	A	12/1995	Clayman et al.
4,989,608	A	2/1991	Ratner	5,483,961	A	1/1996	Kelly et al.
4,991,579	A	2/1991	Allen	5,494,034	A	2/1996	Schlondorff et al.
4,998,938	A	3/1991	Ghajar et al.	5,494,655	A	2/1996	Rocklage et al.
5,006,122	A	4/1991	Wyatt et al.	5,515,160	A	5/1996	Schulz et al.
5,024,236	A	6/1991	Shapiro	5,517,990	A	5/1996	Kalfas et al.
5,027,818	A	7/1991	Bova et al.	5,528,652	A	6/1996	Smith et al.
5,030,223	A	7/1991	Anderson et al.	5,541,377	A	7/1996	Stuhlmacher
5,050,608	A	9/1991	Watanabe et al.	5,572,905	A	11/1996	Cook, Jr.
5,052,329	A	10/1991	Bennett	5,572,999	A	11/1996	Funda et al.
				5,575,798	A	11/1996	Koutrouvelis
				5,618,288	A	4/1997	Calvo et al.

5,622,170 A	4/1997	Schulz	6,482,182 B1	11/2002	Carroll et al.
5,638,819 A	6/1997	Manwaring et al.	6,491,699 B1	12/2002	Henderson et al.
5,643,286 A	7/1997	Warner et al.	6,529,765 B1	3/2003	Franck et al.
5,647,361 A	7/1997	Damadian	6,537,232 B1	3/2003	Kucharczyk et al.
5,649,936 A *	7/1997	Real ..... 606/130	6,546,279 B1	4/2003	Bova et al.
5,658,272 A	8/1997	Hasson	6,547,795 B2 *	4/2003	Schneiderman ..... 606/96
5,662,600 A	9/1997	Watson et al.	6,556,857 B1	4/2003	Estes et al.
5,667,514 A	9/1997	Heller	6,609,020 B2	8/2003	Gill et al.
5,695,501 A	12/1997	Carol et al.	6,632,184 B1	10/2003	Truwit
5,713,858 A	2/1998	Heruth et al.	6,662,035 B2	12/2003	Sochor
5,755,697 A	5/1998	Jones et al.	6,676,669 B2	1/2004	Charles et al.
5,776,064 A	7/1998	Kalfas et al.	6,726,678 B1	4/2004	Nelson et al.
5,776,143 A	7/1998	Adams et al.	6,746,471 B2 *	6/2004	Mortier et al. .... 606/207
5,776,144 A	7/1998	Laysieffer et al.	6,752,812 B1	6/2004	Truwit
5,807,033 A	9/1998	Benway	6,773,443 B2	8/2004	Truwit et al.
5,809,694 A	9/1998	Postans et al.	6,782,288 B2	8/2004	Truwit et al.
5,810,712 A	9/1998	Dunn	6,802,323 B1	10/2004	Truwit et al.
5,817,106 A	10/1998	Real	6,902,569 B2	6/2005	Parmer et al.
5,823,975 A	10/1998	Stark et al.	6,913,478 B2	7/2005	Lamirey et al.
5,833,627 A	11/1998	Shmulewitz et al.	6,944,895 B2	9/2005	Truwit
5,843,150 A	12/1998	Dressen et al.	2001/0014771 A1	8/2001	Truwit et al.
5,851,183 A	12/1998	Bucholz	2001/0027271 A1	10/2001	Franck et al.
5,865,817 A	2/1999	Moening et al.	2001/0037524 A1	11/2001	Truwit
5,865,842 A	2/1999	Knuth et al.	2002/0010479 A1	1/2002	Skakoon et al.
5,871,445 A	2/1999	Bucholz	2002/0019641 A1	2/2002	Truwit
5,871,487 A *	2/1999	Warner et al. .... 606/130	2002/0022847 A1	2/2002	Ray et al.
5,873,822 A	2/1999	Ferre et al.	2002/0052610 A1	5/2002	Skakoon et al.
5,891,034 A	4/1999	Bucholz	2002/0077646 A1	6/2002	Truwit et al.
5,891,157 A	4/1999	Day et al.	2002/0156372 A1	10/2002	Skakoon et al.
5,927,277 A	7/1999	Baudino et al.	2003/0079287 A1	5/2003	Truwit
5,950,629 A	9/1999	Taylor et al.	2003/0187351 A1 *	10/2003	Franck et al. .... 600/429
5,954,687 A	9/1999	Baudino	2004/0059260 A1	3/2004	Truwit
5,957,933 A	9/1999	Yanof et al.	2004/0176750 A1	9/2004	Nelson et al.
5,957,934 A	9/1999	Rapoport et al.	2004/0243147 A1	12/2004	Lipow
5,964,705 A	10/1999	Truwit et al.	2004/0255991 A1	12/2004	Truwit et al.
5,980,535 A	11/1999	Barnett et al.	2004/0260323 A1	12/2004	Truwit et al.
5,984,930 A	11/1999	Maciunas et al.	2004/0267284 A1	12/2004	Parmer et al.
5,993,463 A	11/1999	Truwit	2006/0192319 A1	8/2006	Solar
6,006,126 A	12/1999	Cosman	2006/0195119 A1	8/2006	Mazzocchi et al.
6,018,094 A	1/2000	Fox	2007/0250078 A1	10/2007	Stuart
6,021,343 A	2/2000	Foley et al.	2007/0299427 A1	12/2007	Yeung et al.
6,024,729 A	2/2000	Dehdashtian et al.	2008/0004632 A1	1/2008	Sutherland et al.
6,039,725 A	3/2000	Moening et al.			
6,044,304 A	3/2000	Baudino			
6,058,323 A	5/2000	Lemelson			
6,071,288 A	6/2000	Carol et al.	DE	3937052	5/1990
6,076,008 A	6/2000	Bucholz	DE	29612100	9/1996
6,079,681 A	6/2000	Stern et al.	DE	19726141	1/1999
6,110,182 A	8/2000	Mowlai-Ashtiani	DE	19826078	8/1999
6,117,143 A	9/2000	Hynes et al.	DE	19808220	9/1999
6,120,465 A	9/2000	Guthrie et al.	DE	19820808	11/1999
6,135,946 A	10/2000	Konen et al.	EP	0386936	9/1990
6,179,826 B1	1/2001	Aebischer et al.	EP	0427358	5/1991
6,195,577 B1	2/2001	Truwit et al.	EP	0609085	8/1994
6,206,890 B1	3/2001	Truwit	EP	0724865	8/1996
6,210,417 B1	4/2001	Baudino et al.	EP	0832611	4/1998
6,231,526 B1	5/2001	Taylor et al.	EP	0904741	3/1999
6,236,875 B1	5/2001	Bucholz et al.	GB	2237993	5/1991
6,254,532 B1	7/2001	Paolitto et al.	GB	2329473	3/1999
6,257,407 B1	7/2001	Truwit et al.	GB	2346573	8/2000
6,261,300 B1	7/2001	Carol et al.	WO	WO-8809151	12/1988
6,267,769 B1	7/2001	Truwit	WO	WO-9522297	8/1995
6,267,770 B1	7/2001	Truwit	WO	WO-9610368	4/1996
6,273,896 B1	8/2001	Franck et al.	WO	WO-9633766	10/1996
6,282,437 B1	8/2001	Franck et al.	WO	WO-9703609	2/1997
6,290,644 B1	9/2001	Green, II et al.	WO	WO-9721380	6/1997
6,298,262 B1	10/2001	Franck et al.	WO	WO-9742870	11/1997
6,315,770 B1	11/2001	de la Torre et al.	WO	WO-9817191	4/1998
6,321,104 B1	11/2001	Gielen et al.	WO	WO-9825535	6/1998
6,327,491 B1	12/2001	Franklin et al.	WO	WO-9851229	11/1998
6,356,792 B1	3/2002	Errico et al.	WO	WO-0001316	1/2000
6,368,329 B1	4/2002	Truwit	WO	WO-0018306	4/2000
6,457,963 B1	10/2002	Tawara et al.	WO	WO-0124709	4/2001

FOREIGN PATENT DOCUMENTS

WO WO-0149197 7/2001  
 WO WO-0176498 10/2001

## OTHER PUBLICATIONS

- “CRWTM—Tyco Healthcare Radionics”, *Tyco Products Brochure*, pp. 1-7.
- “Fathom Remote Introducer”, *Image-Guided Neurologics, Inc.*, CNS Hynes Convention Center, (Oct. 30-Nov. 4, 1999), 2 pgs.
- “Inomed Competence in Neurophysiologic Monitoring”, <http://www.inomed.com/english/index.htm>, (observed Mar. 23, 2004), 2 pgs.
- “Leksell Stereotaxic System”, *Elekta Products Brochure*, pp. 1-6.
- “MicroTargeting® Precision Guidance Using Microelectrode Recording”, (Aug. 15, 2003), 5 pgs.
- “Possible Existence of Common Internalization Mechanisms among Arginine-rich Peptides”, Suzuki, T. et al., *Journal of Biological Chemistry*, vol. 277, No. 4 (2002) pp. 2437-2443.
- Allison, S., et al., “Microchannel Plate Intensifier Response in Traverse Magnetic Field”, *Electronic Letters*, 26, (Jun. 7, 1990), 770-771.
- Drake, J. M., et al., “ISG Viewing Wand System”, *Neurosurgery*, 34 (6), (Jun. 1994), pp. 1094-1097.
- Dyer, P. V., et al., “The ISG Viewing Wand: an application to atlanto-axial surgery using the Le Fort I maxillary osteotomy”, *British Journal of Oral & Maxillofacial Surgery*, 33, (1995), pp. 370-374.
- Franck, Joel, et al., “microTargeting® Platform incorporating StarFix™ guidance”, *microTargeting*, 3 pgs.
- Franck, Joel, et al., “microTargeting® Platform System incorporating StarFix™ guidance”, *microTargeting*, p. 44.
- Gehring, W. J., “Homeodomain Proteins”, *Annu. Rev. Biochem.*, vol. 63 (1997) pp. 487-526.
- Gillies, G., et al., “Magnetic Manipulation Instrumentation for Medical Physics Research”, *Review of Scientific Instruments*, 65 (3), Review Article, (Mar. 1994), 533-562.
- Grady, M. S., “Magnetic Stereotaxis System for Neurosurgical Procedures”, *Proceedings of the 37th International Instrumentation Symposium*, (May 5-9, 1991), pp. 665-675.
- Grady, M. S., et al., “Initial Experimental Results of a New Stereotaxic Hyperthermia System”, *American College of Surgeons, Surgical Forum*, vol. XXXIX, *Neurological Surgery*, (1988), pp. 507-509.
- Grady, M. S., et al., “Magnetic Stereotaxis: A Technique to Deliver Stereotactic Hyperthermia”, *Neurosurgery*, 27 (6), (1990), pp. 1010-1016.
- Grady, M. S., et al., “Preliminary experimental investigation of in vivo magnetic manipulation: Results and potential application in hyperthermia”, *Medical Physics*, 16 (2), (Mar./Apr. 1989), pp. 263-272.
- Grady, M., et al., “Nonlinear Magnetic Stereotaxis: Three-Dimensional, in vivo Remote Magnetic Manipulation of a Small Object in Canine Brain”, *Medical Physics*, 17 (3), (May/June 1990), pp. 405-415.
- Hata, N., et al., “Needle Insertion Manipulator for CT- and MR-Guided Stereotactic Neurosurgery”, *Interventional MR: Techniques and Clinical Experience*, St. Louis: London: Mosby; Martin Dunitz, F. Jolesz and I. Young, eds., (1998), pp. 99-106.
- Hirschberg, H., et al., “Image-guided neurosurgery—MR compatible stereotactic equipment”, <http://www.medinnova.no/English/P51466ster.html>, (Mar. 29, 2001), 1 pg. (viewed website on Mar. 29, 2001).
- Hirschberg, Henry, et al., “Image-guided neurosurgery”, stereotactic equipment for MR imaging, <http://www.medinnova.no/English/P51466ster.html>, (Observed Mar. 8, 2002), 1 page.
- Howard III, M. A., et al., “Magnetic Neurosurgery: Image-Guided Remote-Controlled Movement of Neurosurgical Implants”, *Clinical Neurosurgery*, (1995), pp. 382-391.
- Howard III, M. A., et al., “Review of Magnetic Neurosurgery Research”, *Journal of Image Guided Surgery*, 1 (6), (1995), pp. 295-299.
- Howard, M. A., et al., “Magnetic Movement of a Brain Thermoceptor”, *Neurosurgery*, 24 (3), (Mar. 1989), pp. 444-448.
- Howard, M. A., et al., “Magnetic Neurosurgery”, *Proceedings of the Meeting of the American Society for Stereotactic and Functional Neurosurgery*, (Mar. 8-11, 1995), pp. 102-107.
- Lawson, M. A., et al., “Near Real-Time Bi-planar Fluoroscopic Tracking System for the Video Tumor Fighter”, *SPIEvol. 1445 Image Processing*, (1991), pp. 265-275.
- Leggett, W.B., et al., “Surgical Technology—The Viewing Wand: A New System for Three-Dimensional Computed Tomography-Correlated Intraoperative Localization”, *Current Surgery*, (Dec. 1991), pp. 674-678.
- Malison, R. T., et al., “Computer-Assisted Coregistration of Multislice SPECT and MR Brain Images by Fixed External Fiducials”, *Journal of Computer Assisted Tomography*, 17 (6) (1993) pp. 952-960.
- Mannervik, M., “Target genes of homeodomain proteins”, *BioEssays* vol. 21.4 (Apr. 1999) pp. 267-270.
- McNeil, R. G., et al., “Characteristics of an Improved Magnetic-Implant Guidance System”, *IEEE Transactions on Biomedical Engineering*, 42 (8), (Aug. 1995), pp. 802-808.
- McNeil, R. G., et al., “Functional Design Features and Initial Performance Characteristics of a Magnetic-Implant Guidance System for Stereotactic Neurosurgery”, *IEEE Transactions on Biomedical Engineering*, 42 (8), pp. 793-801.
- Meeker, D., et al., “Optimal Realization of Arbitrary Forces in a Magnetic Stereotaxis System,” *IEEE Transactions on Magnetics*, 32 (2), (Mar. 1996), 320-328.
- Molloy, J. A., et al., “Experimental Determination of the Force Required for Insertion of a Thermoseed Into Deep Brain Tissues”, *Annals of Biomedical Engineering*, 18 (3), (1990), pp. 299-313.
- Molloy, J. A., et al., “Thermodynamics of movable inductively heated seeds for the treatment of brain tumors”, *Medical Physics*, 18 (4), (Jul./Aug. 1991), pp. 794-803.
- Oliver, L., “Cup-And-Ball Chemopallidectomy Apparatus”, (1958), p. 104.
- Patikoglou, G. et al., “Eukaryotic Transcription Factor-DNA Complexes”, *Annual Review of Biophysics and Biomolecular Structure* vol. 26 (1997) pp. 289-325.
- Quate, E., et al., “Goniometric Motion Controller for the Superconducting Coil in a Magnetic Stereotaxis System”, *IEEE Transactions on Biomedical Engineering*, 38 (9), (Sep. 1991), 899-905.
- Ramos, P. A., et al., “Electro-optic imaging chain for a biplanar fluoroscope for neurosurgery: magnetic field sensitivity and contrast measurements”, *Optical Engineering*, 32 (7), (Jul. 1993), pp. 1644-1656.
- Ramos, P. A., et al., “Low-dose, magnetic field-immune, bi-planar fluoroscopy for neurosurgery”, *SPIE Medical Imaging V: Image Physics*, vol. 1443, (1991), pp. 160-170.
- Ramos, P. A., et al., “Microchannel Plate Image Intensifier Electron Dynamics in Magnetic Field”, *Electronics Letters*, 27 (18), (Aug. 29, 1991), pp. 1636-1638.
- Ritter, R. C., et al., “Magnetic Stereotaxis: An Application of Magnetic Control Technology to the Needs of Clinical Medicine”, *Proc. Of the MAG-95 Industrial Conf. and Exhibition*, Technomic Pub. Co., Lancaster, PA., Allaire, P., ed., (1995), pp. 186-193.
- Ritter, R. C., et al., “Magnetic Stereotaxis: Computer-Assisted Image-Guided Remote Movement of Implants in the Brain”, *Computer-Integrated Surgery: Technology and Clinical Applications*, MIT Press, (1996), pp. 363-369.
- Sandeman, D. S., et al., “Advances in image-directed neurosurgery: Preliminary experience with the ISG Viewing Wand compared with the Leksell G frame”, *British Journal of Neurosurgery*, 8, (1999), pp. 529-544.
- Stein, S. et al., “Checklist: Vertebrate homeobox genes”, *Mechanisms of Development*, vol. 55, No. 1 (Mar. 1996) pp. 91-108.
- Szikora, Istvan, et al., “Endovascular Treatment of Experimental Aneurysms with Liquid Polymers: The Protective Potential of Stents”, *Neurosurgery*, 38 (2), (Feb. 1996), pp. 339-347.
- Vollmer, J. et al., “Homeobox Genes in the Developing Mouse Brain”, *Journal of Neurochemistry*, vol. 71, No. 1 (Jul. 1998) pp. 1-19.

Wolberger, C., "Homeodomain Interactions", *Current Opinion in Structural Biology* vol. 6, No. 1 (Feb. 1996) pp. 62-68.

Yeh, H.-S., et al., "Implantation of intracerebral depth electrodes for monitoring seizures using the Pelorus stereotactic system guided by magnetic resonance imaging", *J. Neurosurg.*, 78, (1993), pp. 138-141.

Zinreich, S. J., et al., "Frameless Stereotaxic Integration of CT Imaging Data: Accuracy and Initial Applications", *Radiology*, 188 (3), (1993), pp. 735-742.

International Search Report and Written Opinion for PCT/US05/43651 mailed May 8, 2008.

\* cited by examiner

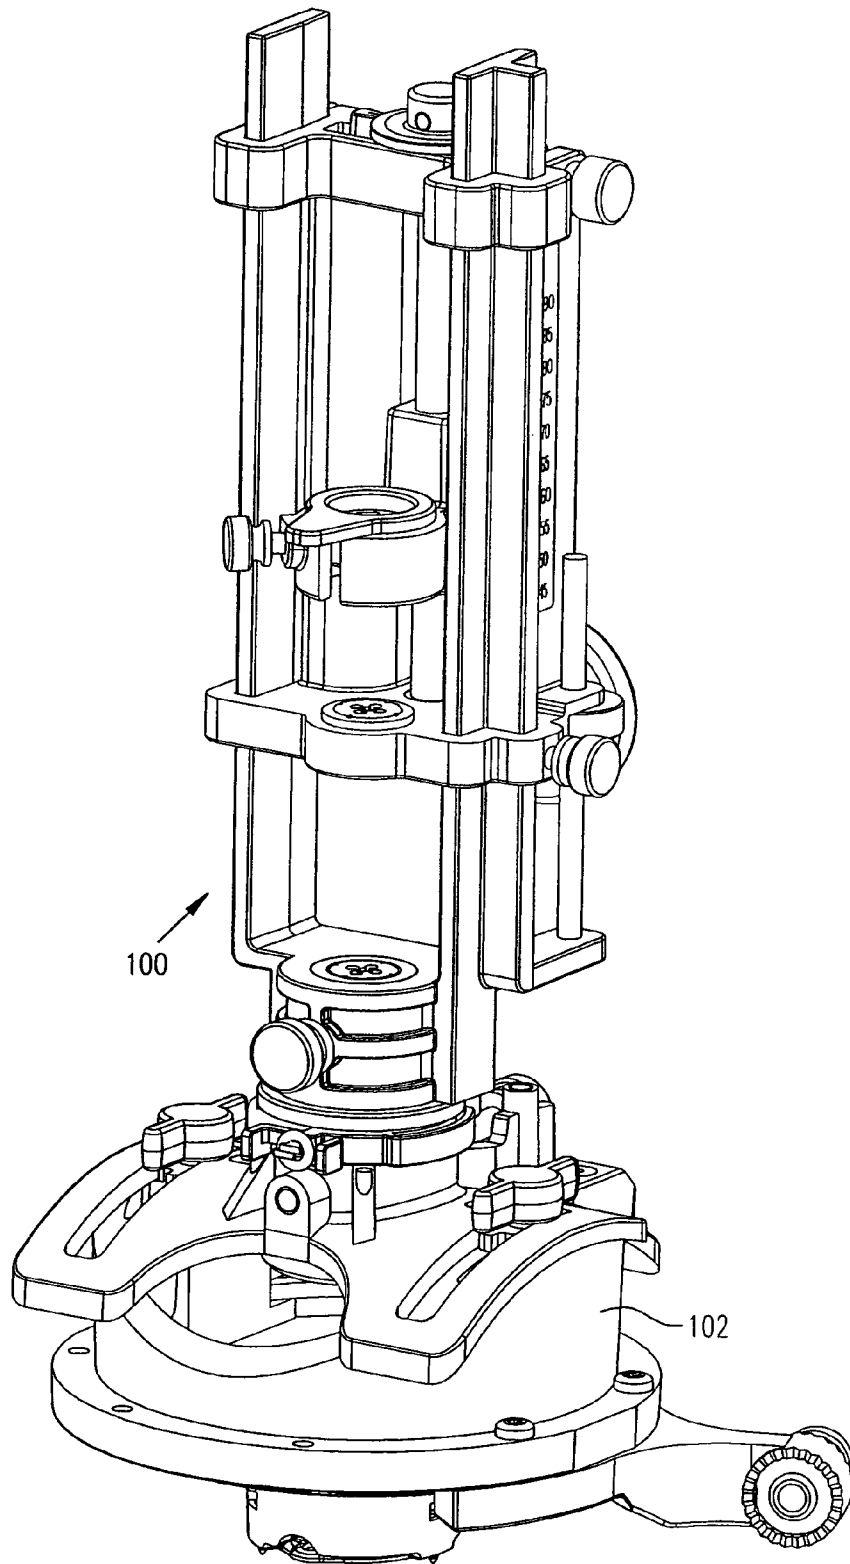


FIG. 1

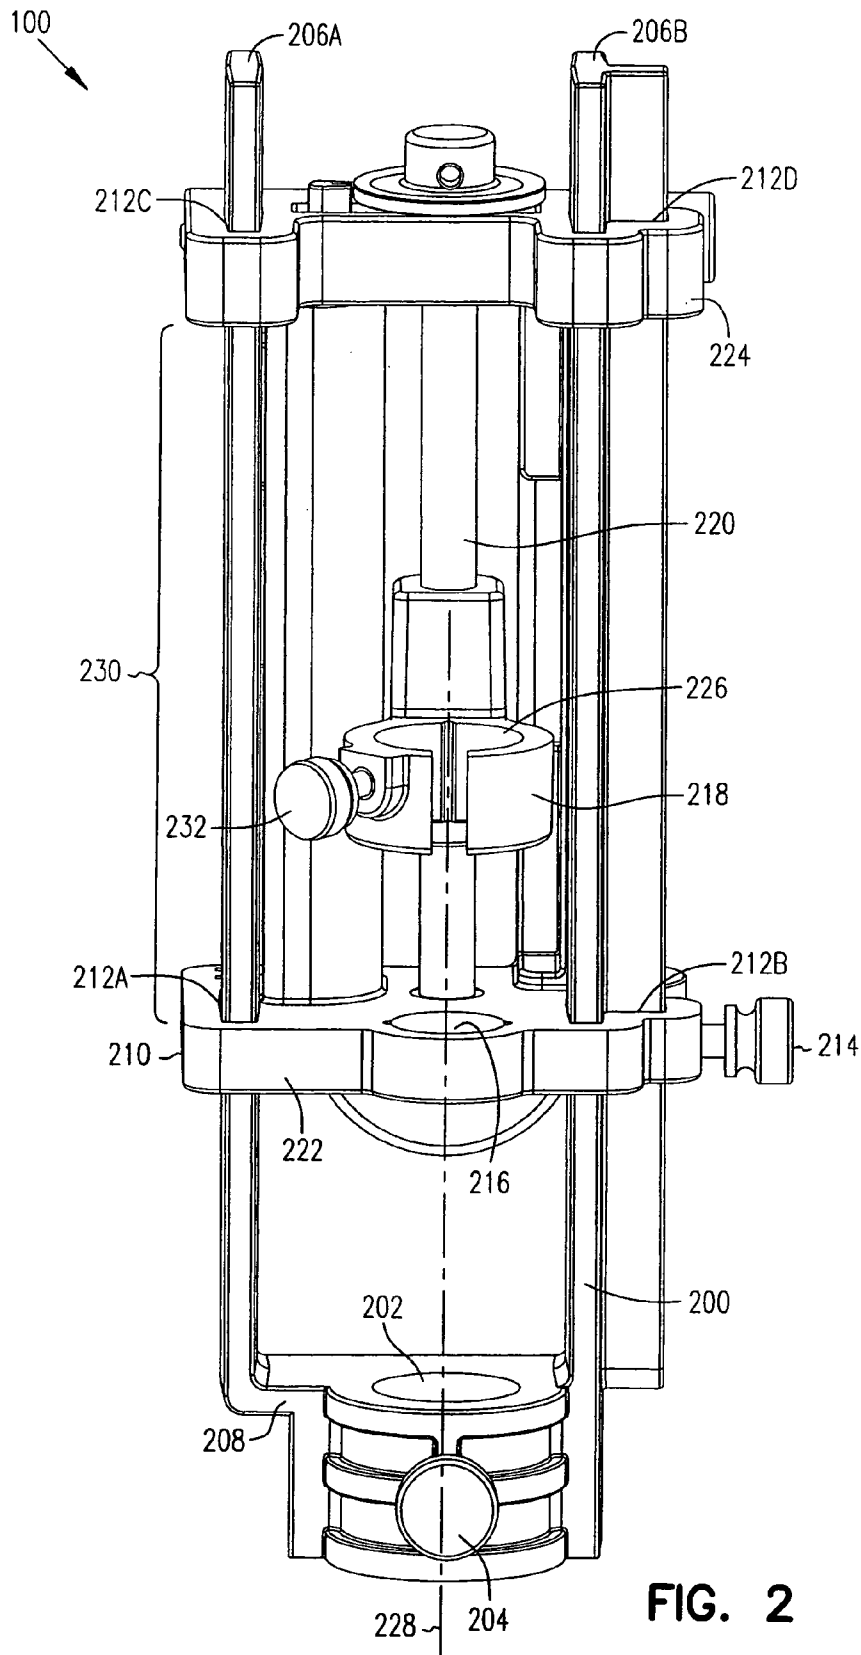


FIG. 2

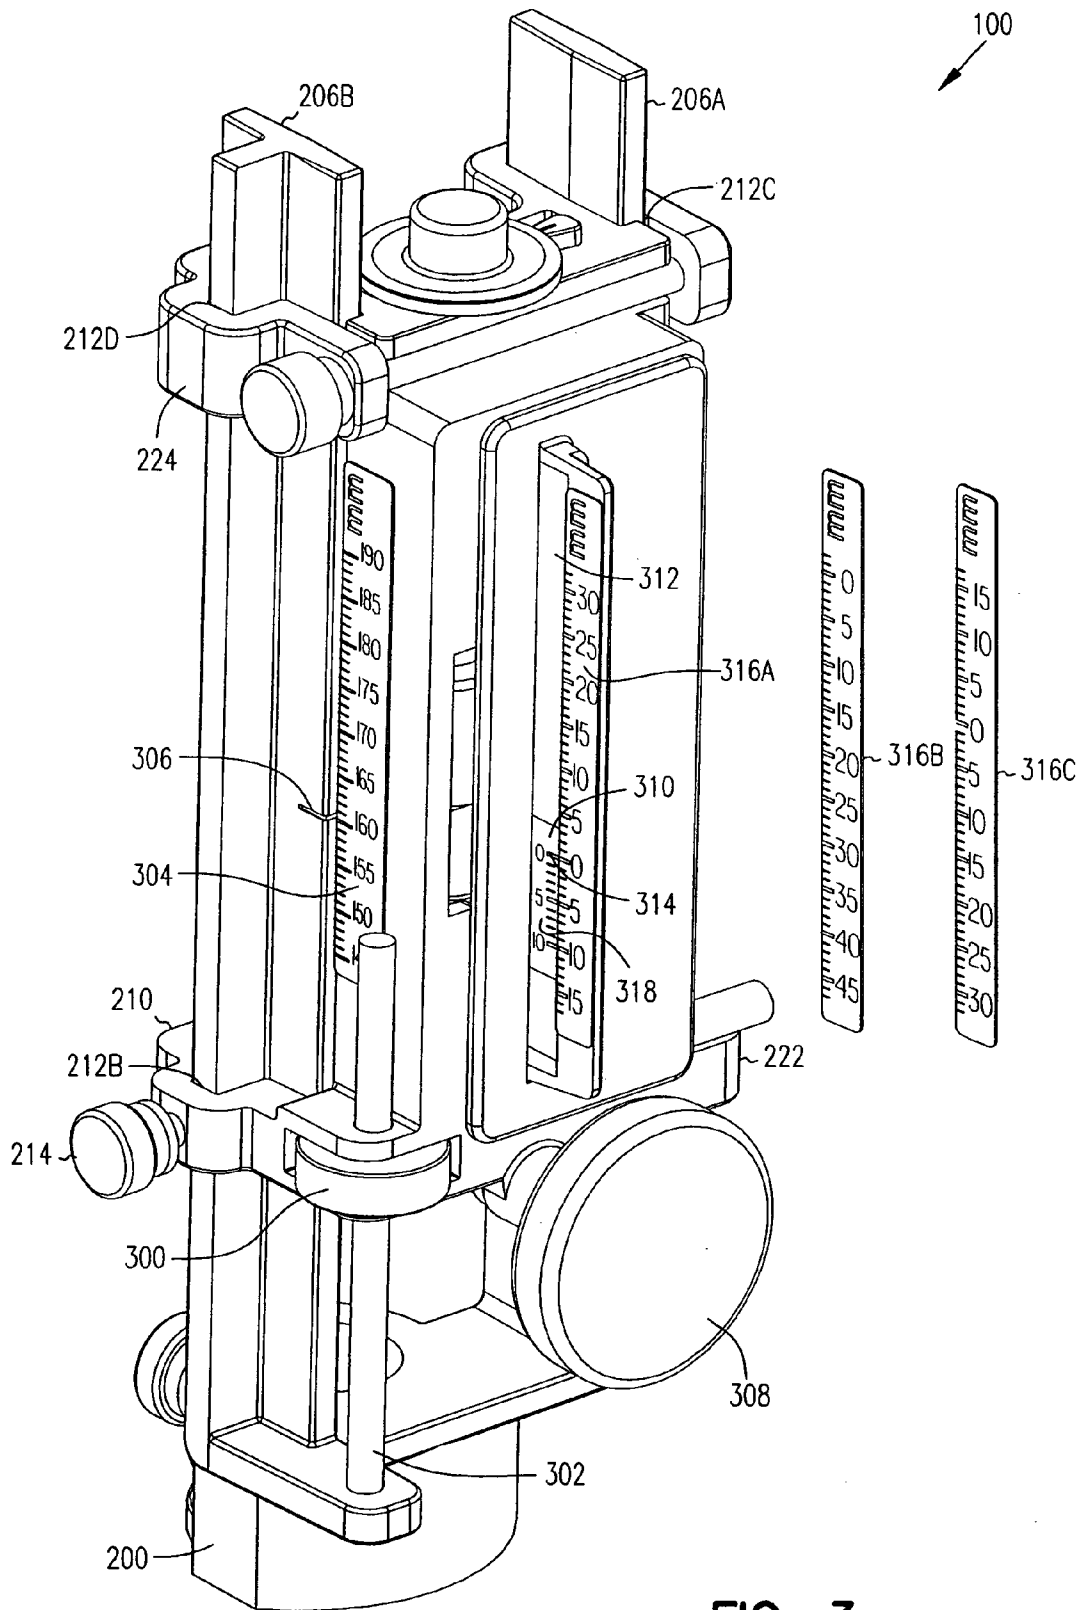


FIG. 3



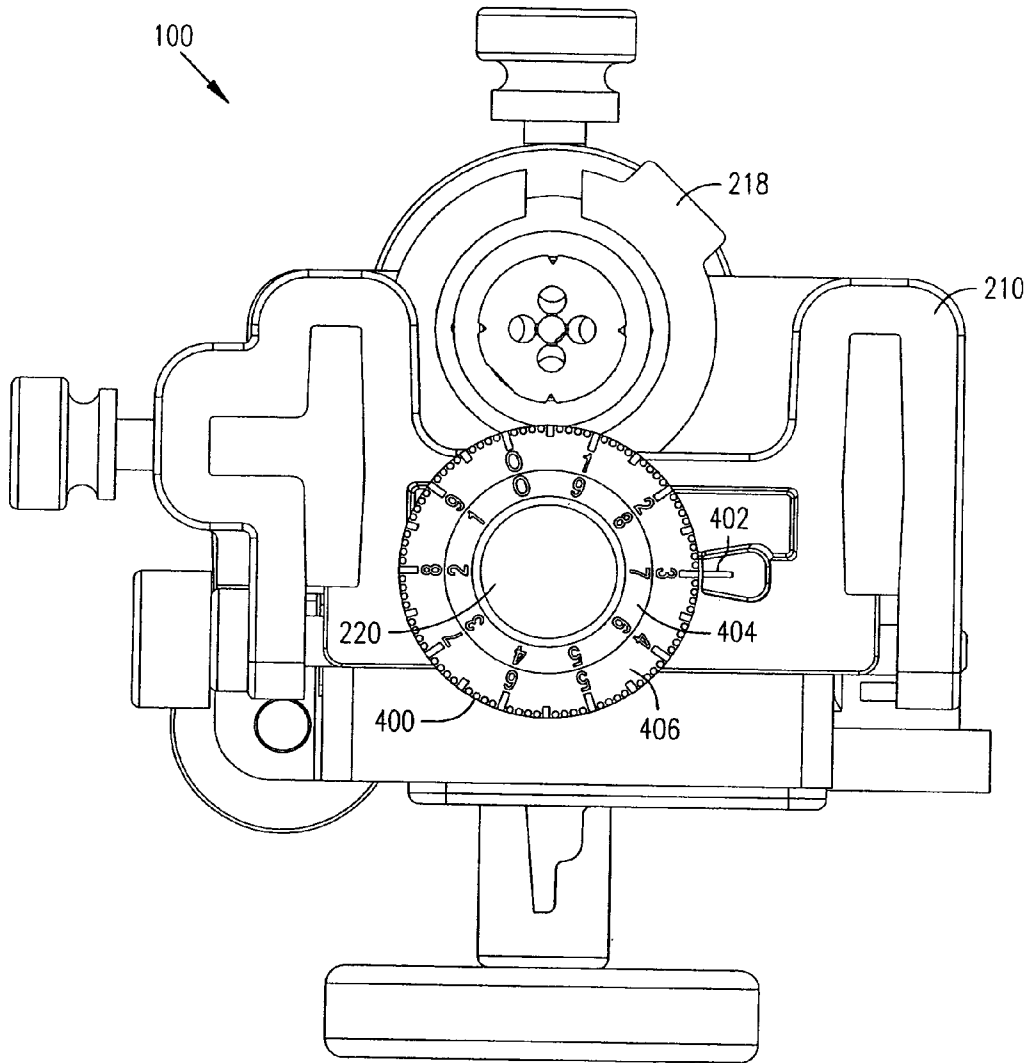


FIG. 4

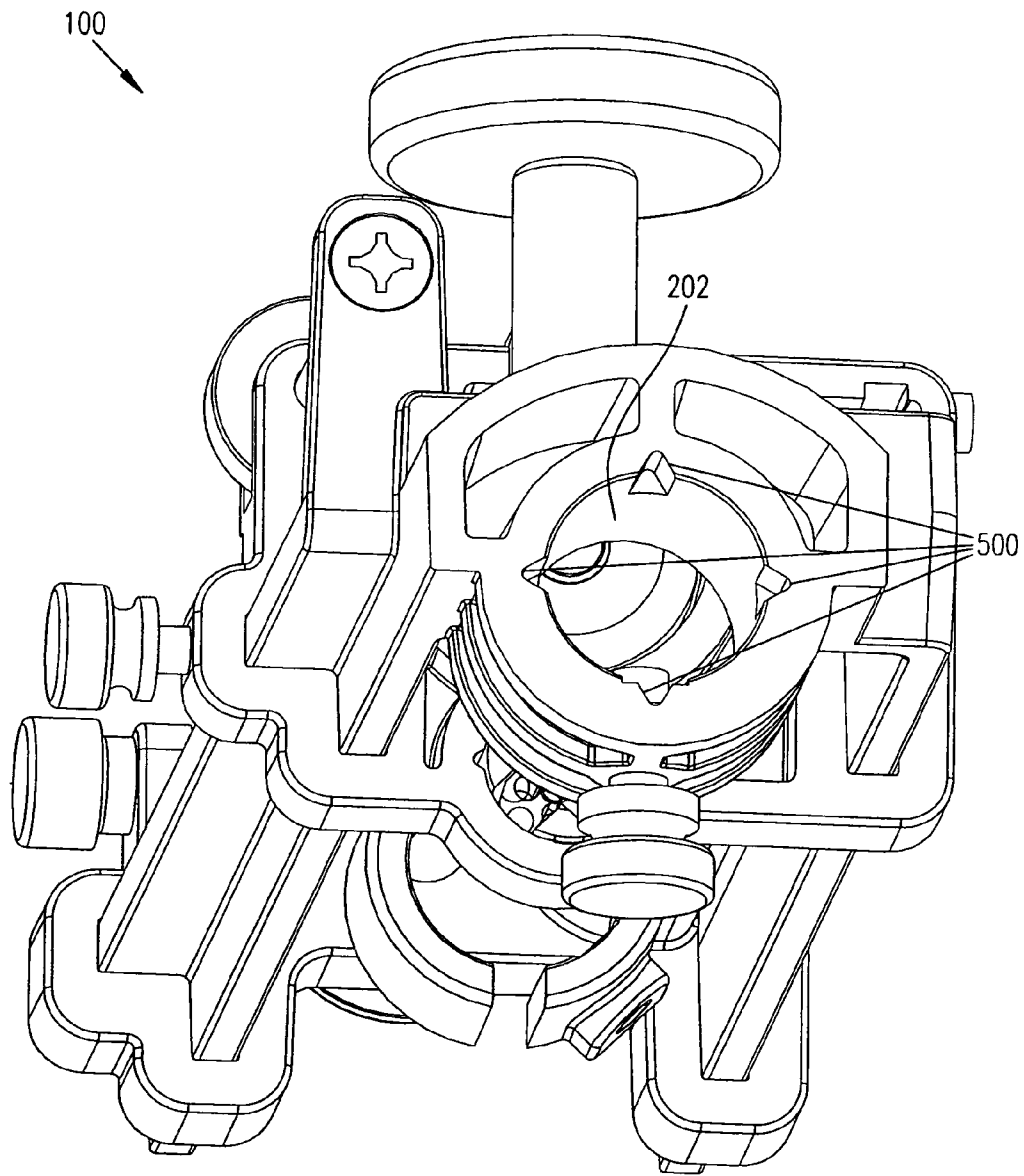


FIG. 5

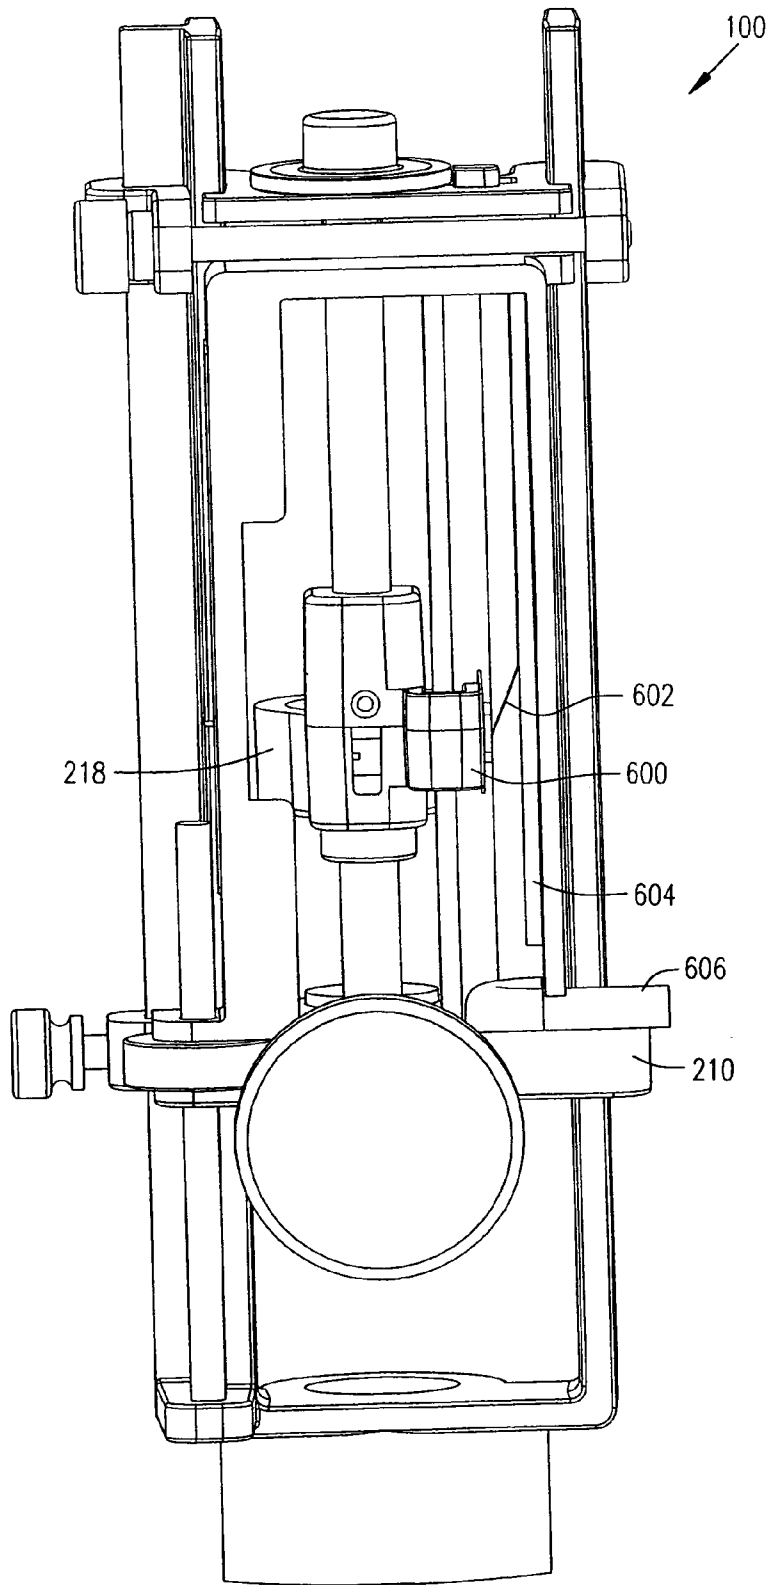


FIG. 6

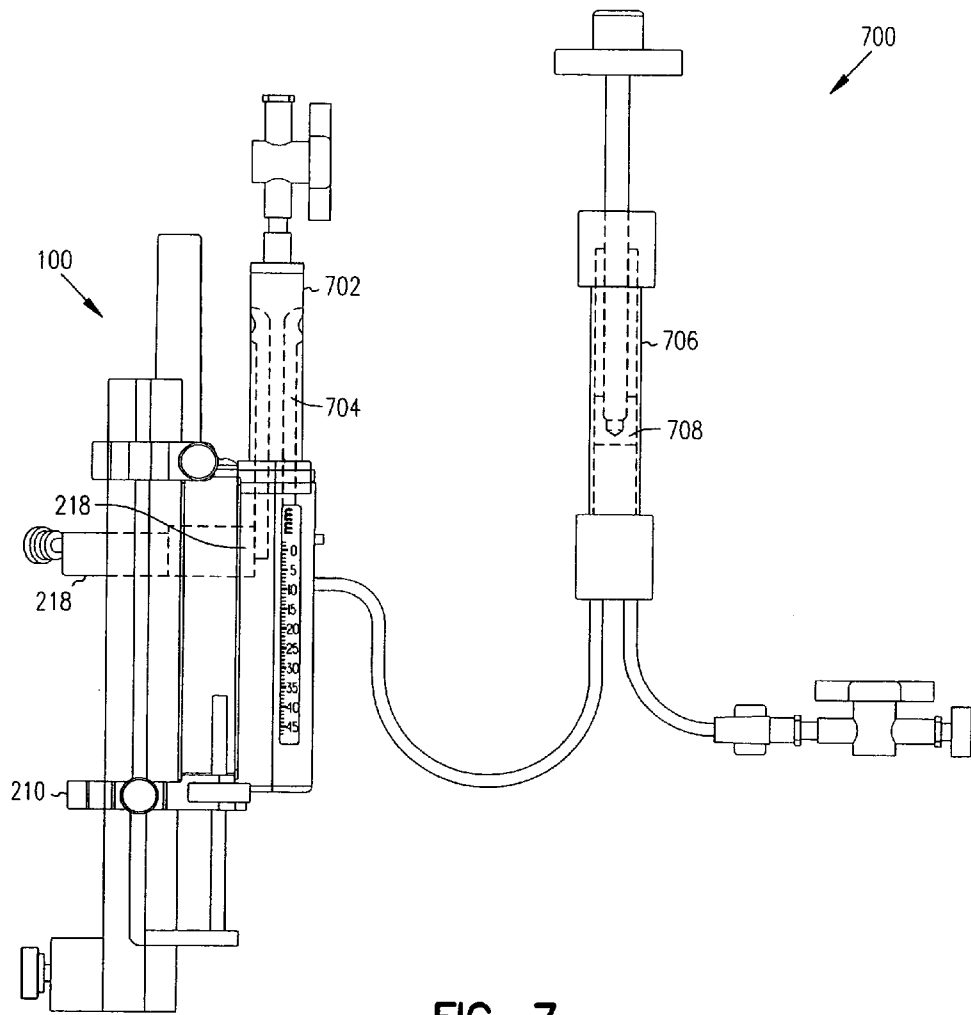
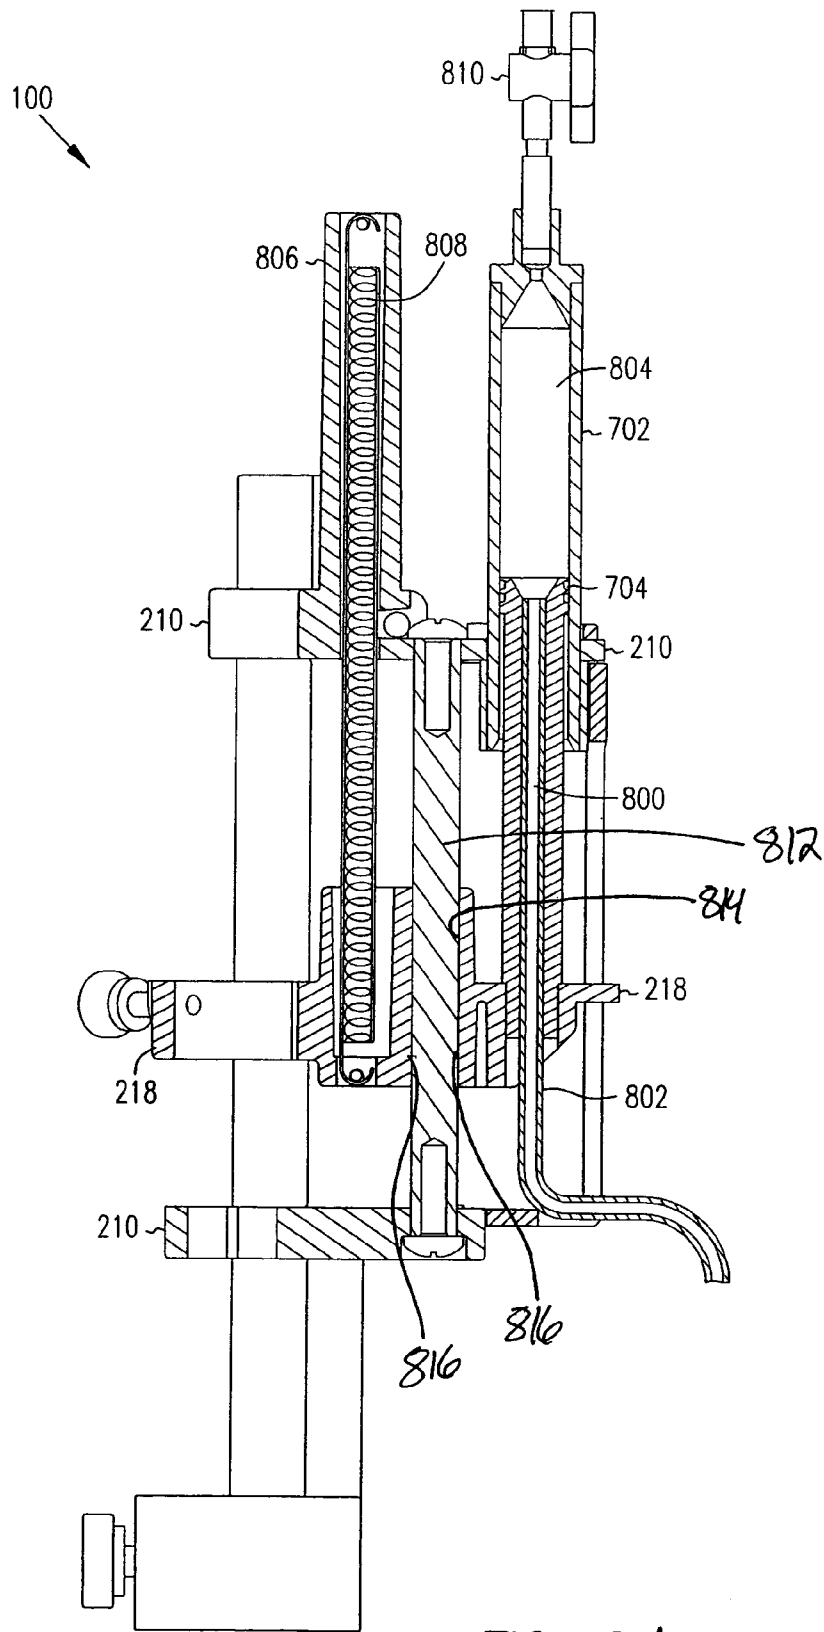


FIG. 7



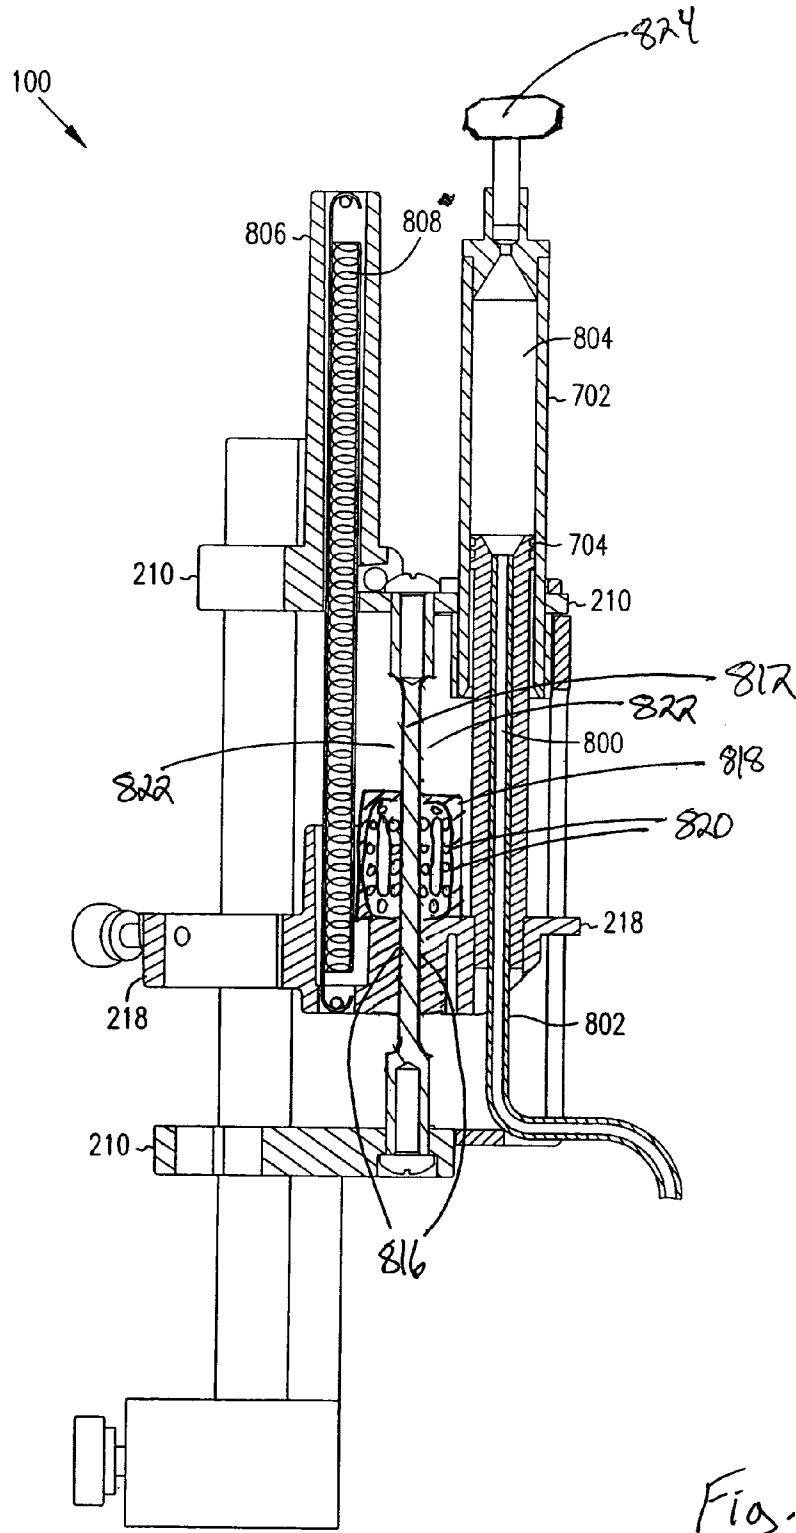
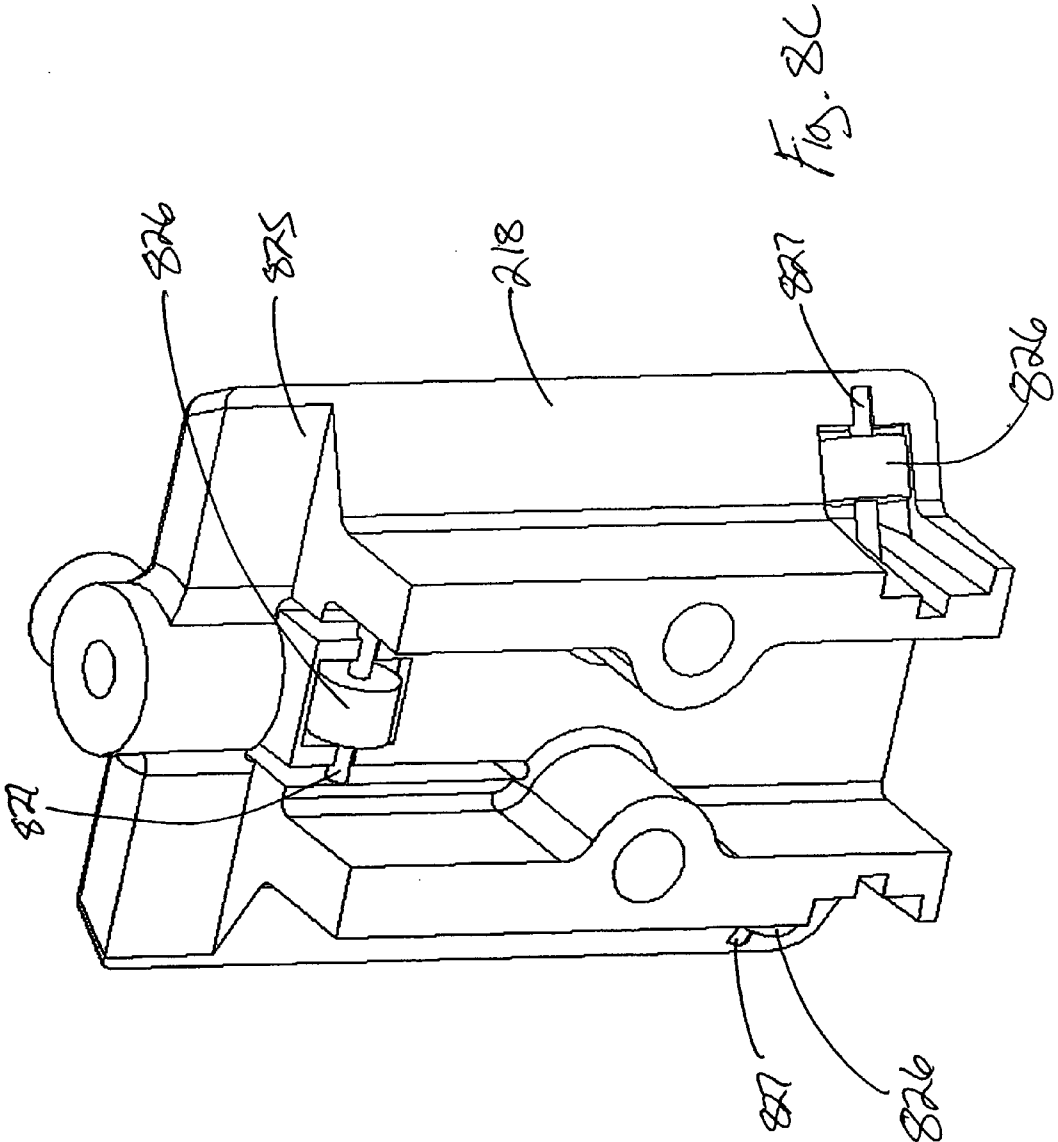


Fig. 8B



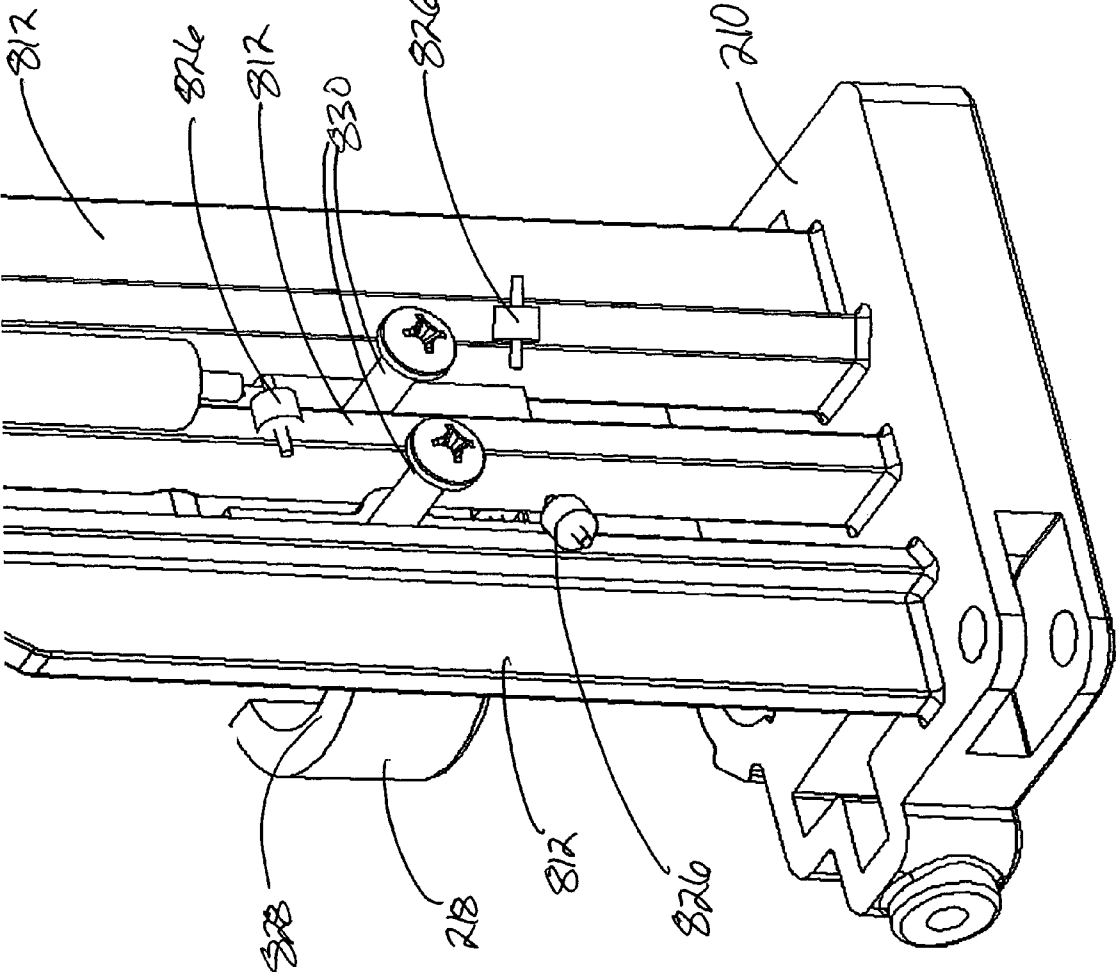
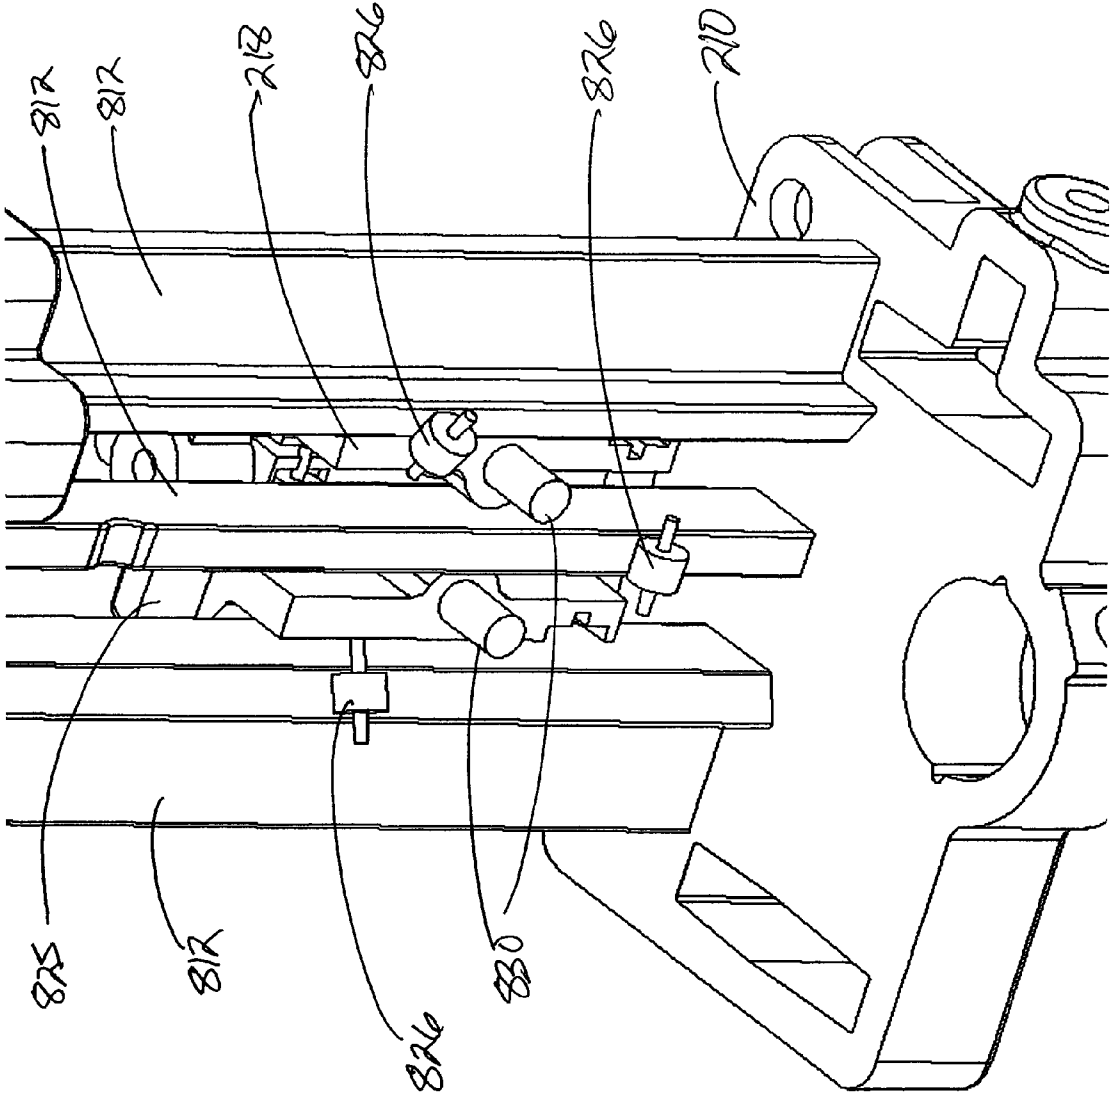


FIG. 8D



Fig. 2E



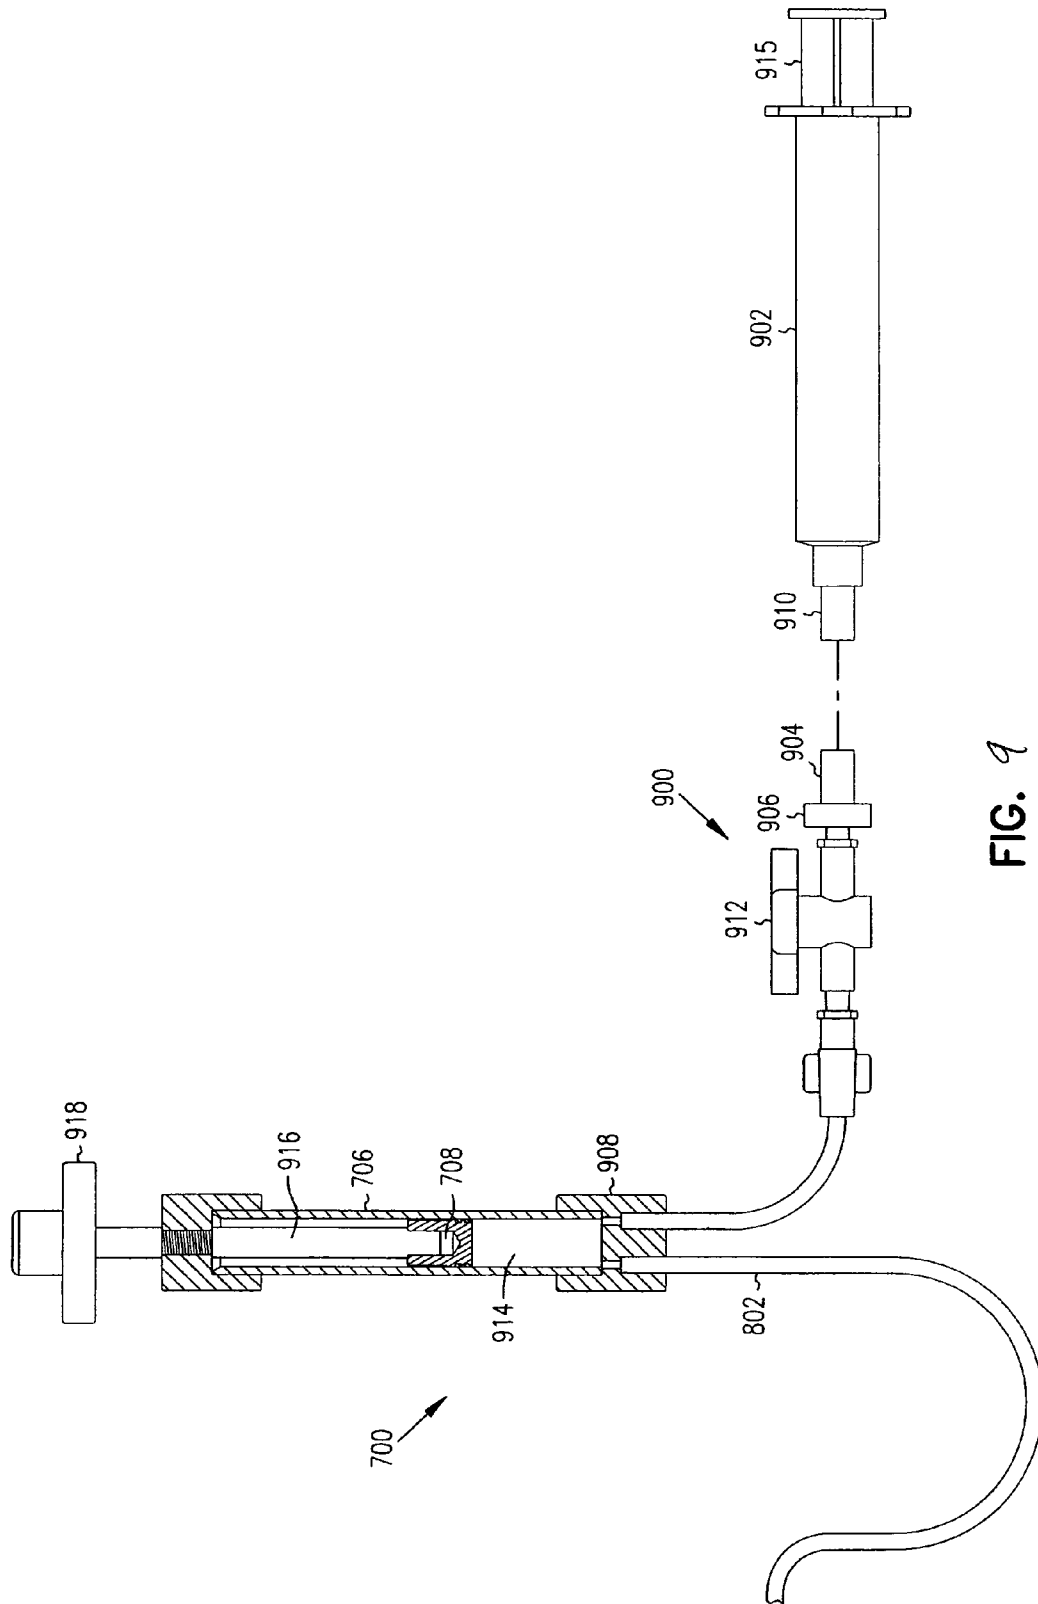


FIG. 9

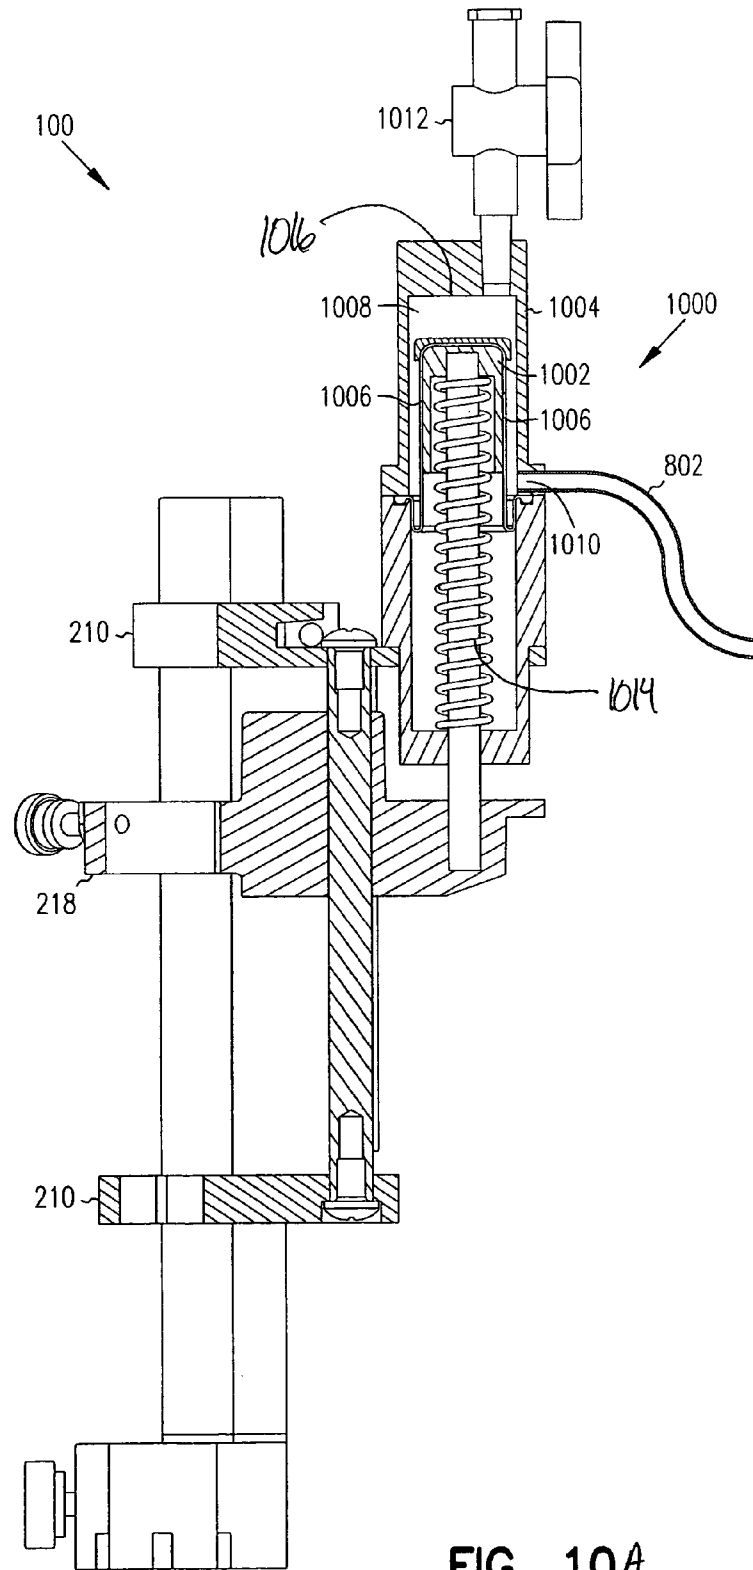


FIG. 10A

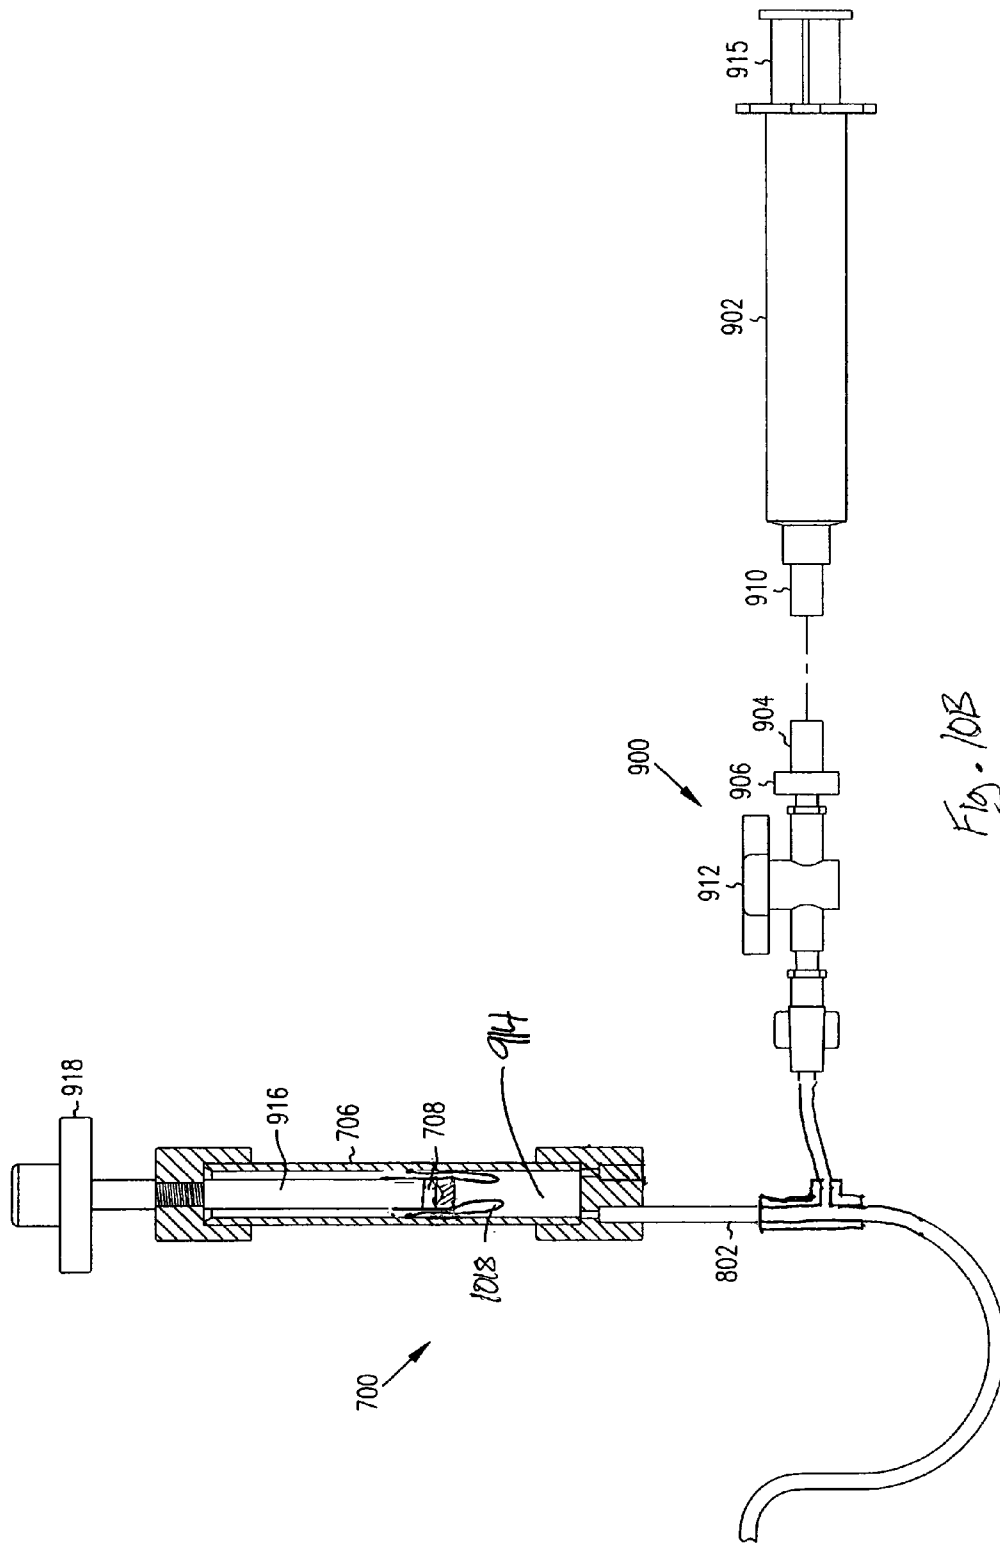


Fig. 10B

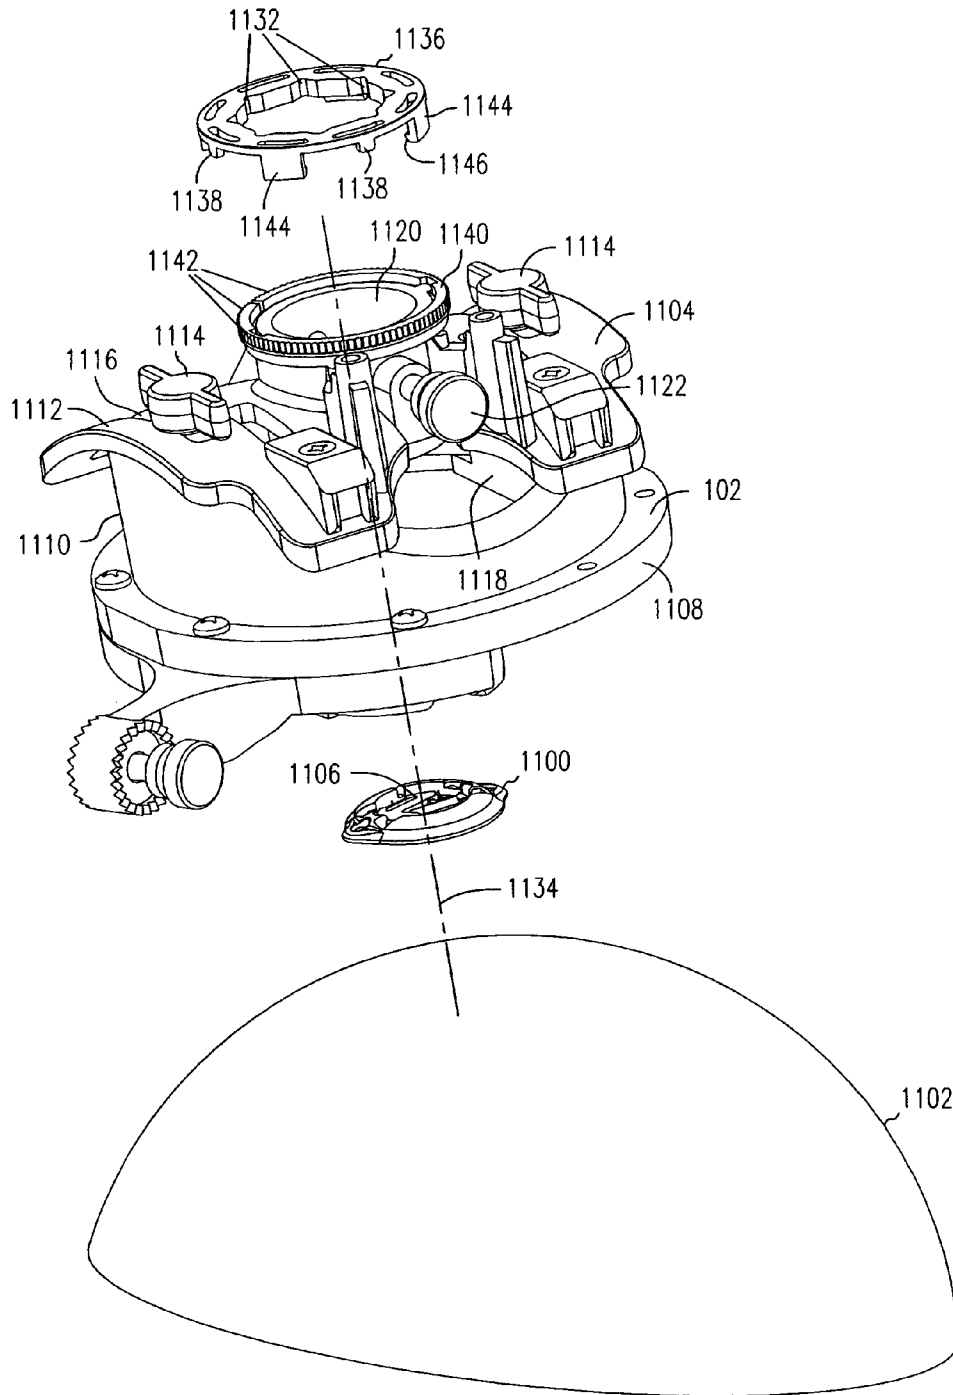


FIG. 11A

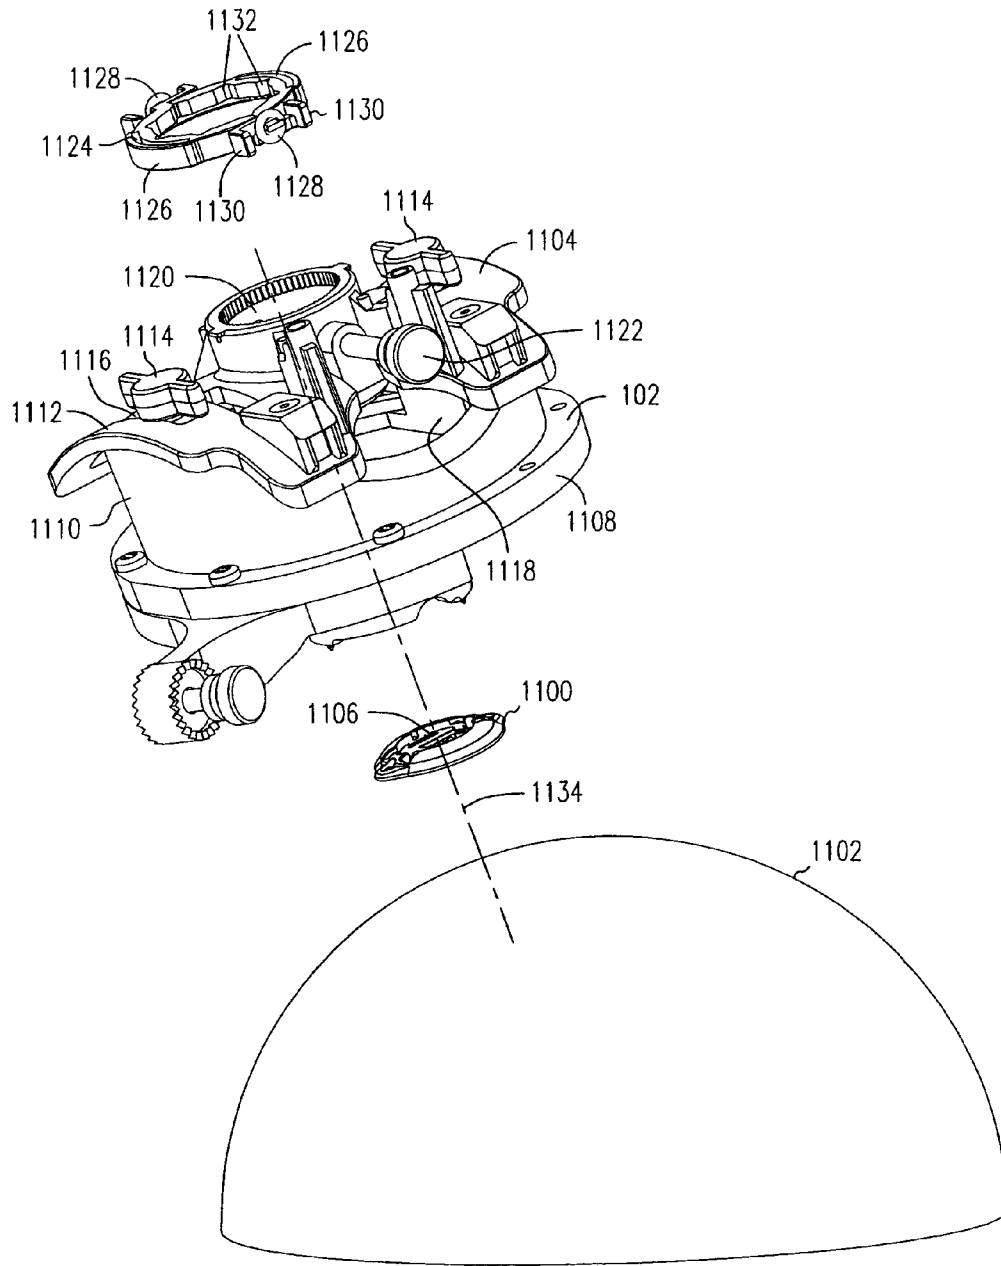


FIG. 11B

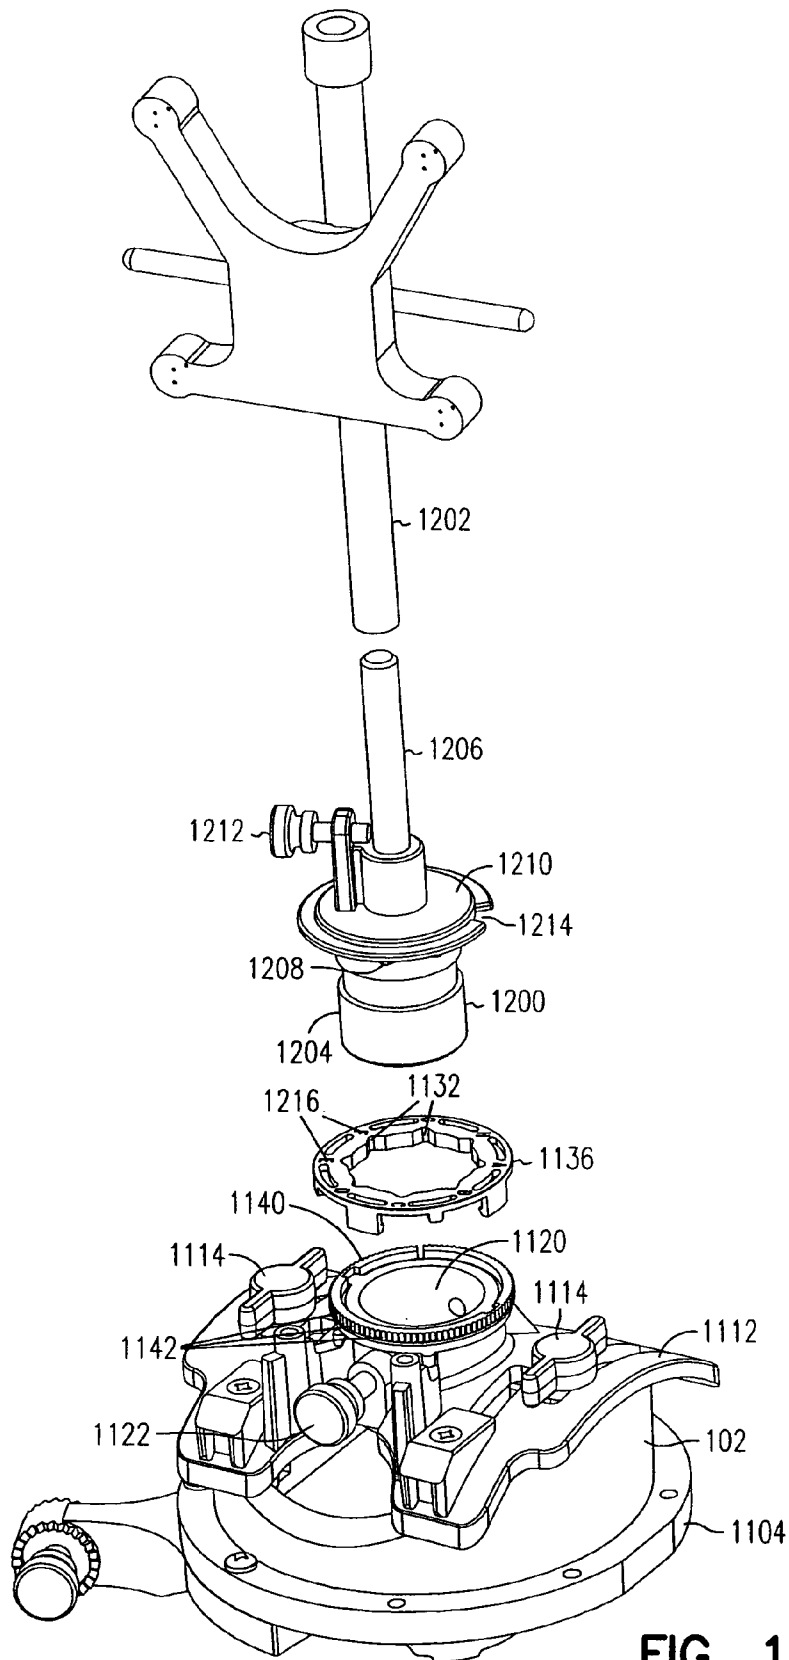


FIG. 12

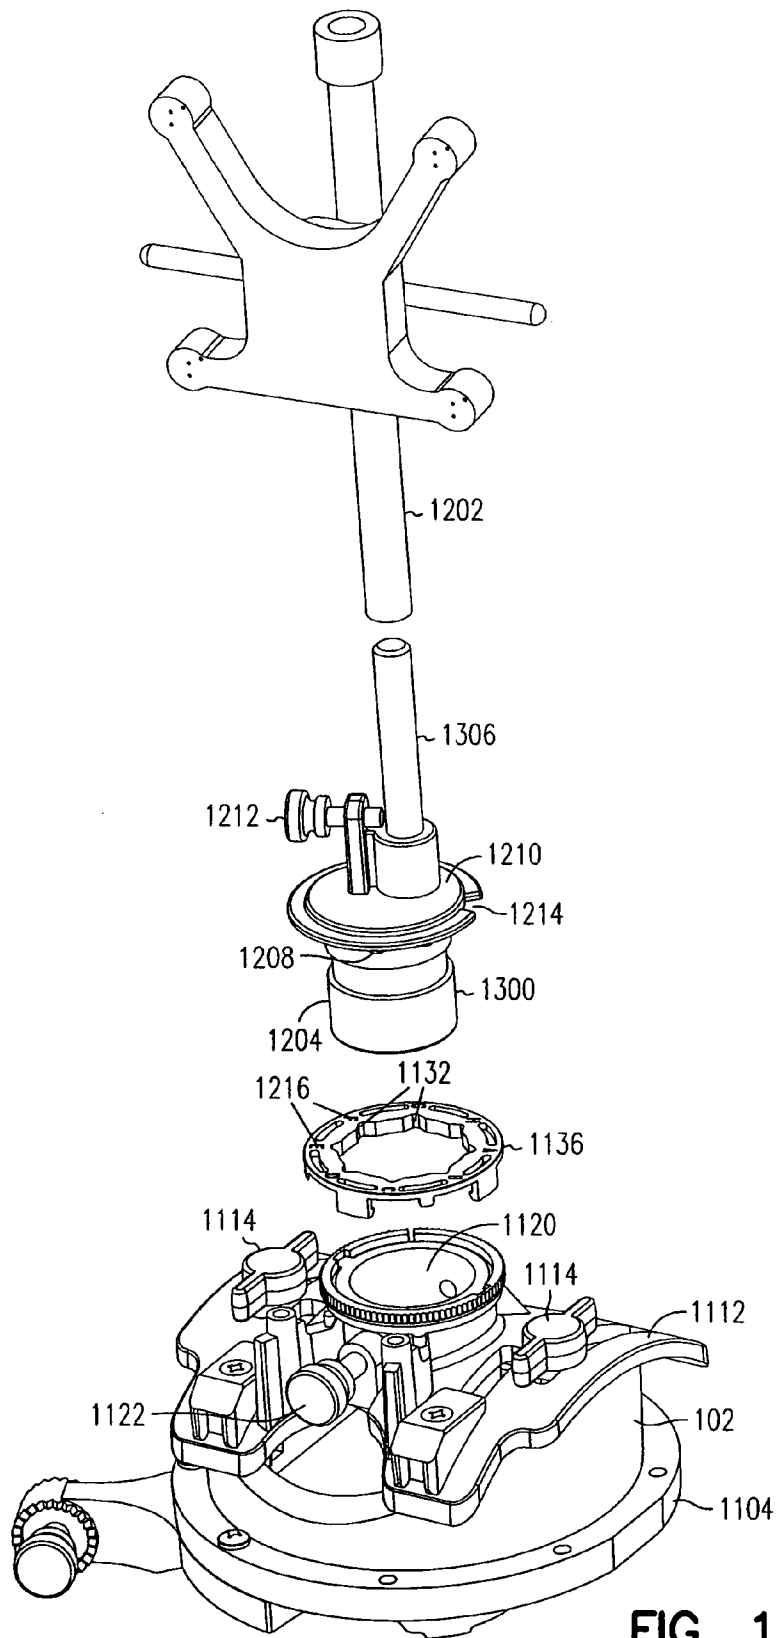


FIG. 13



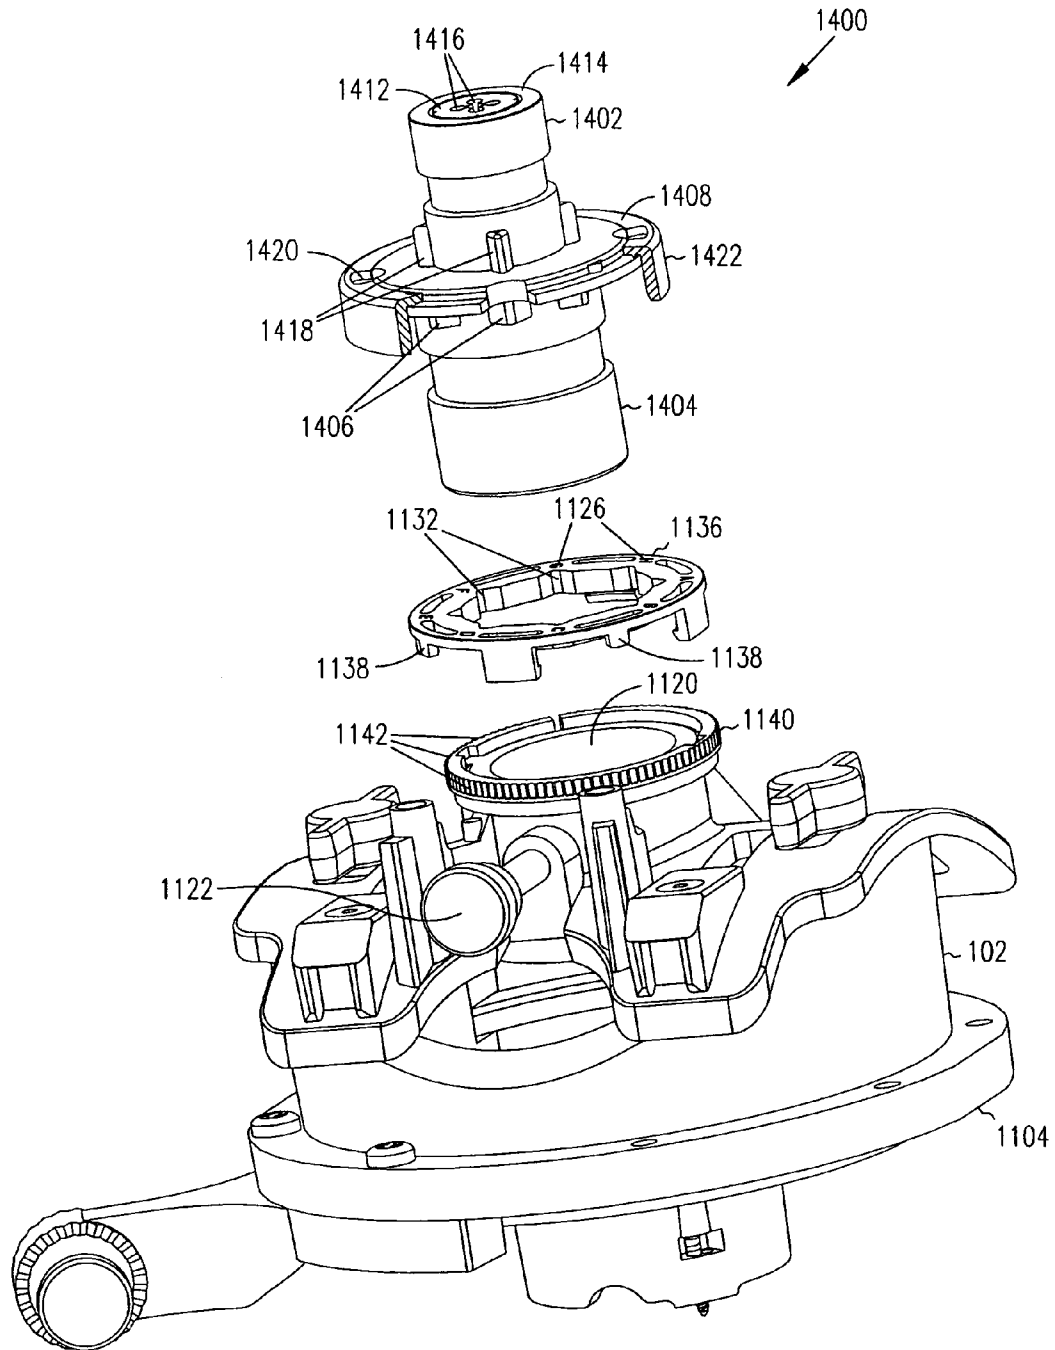


FIG. 14

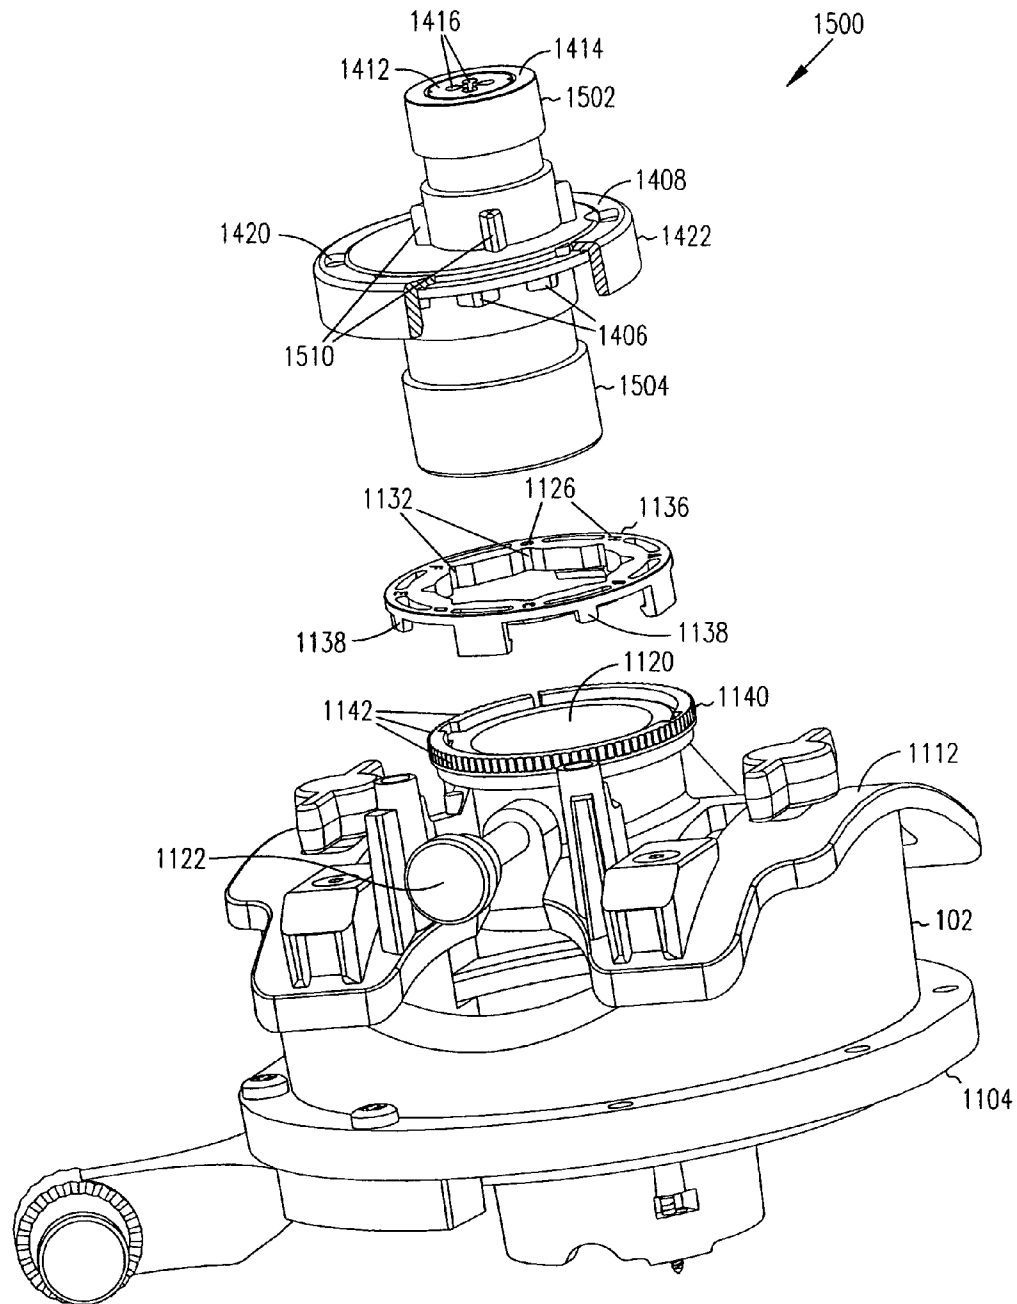


FIG. 15

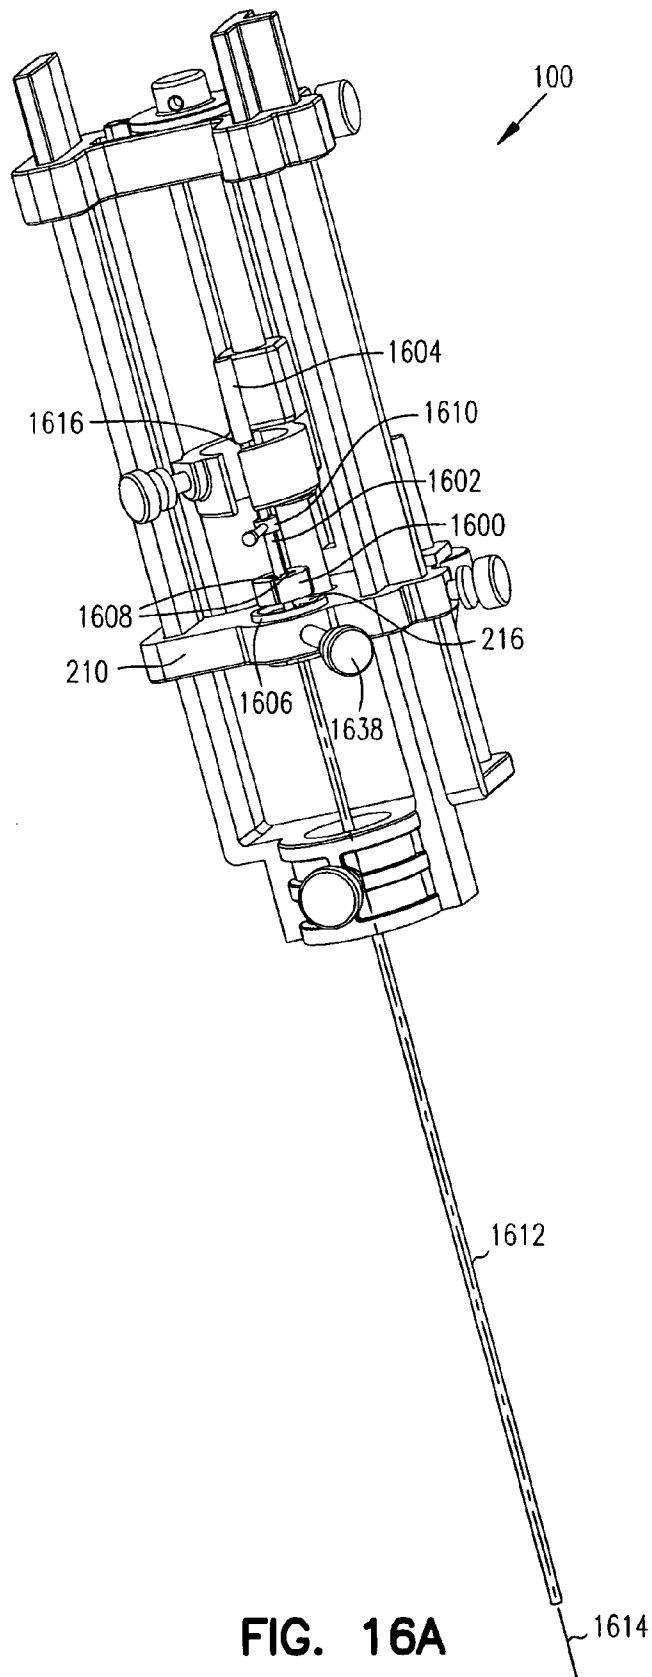


FIG. 16A

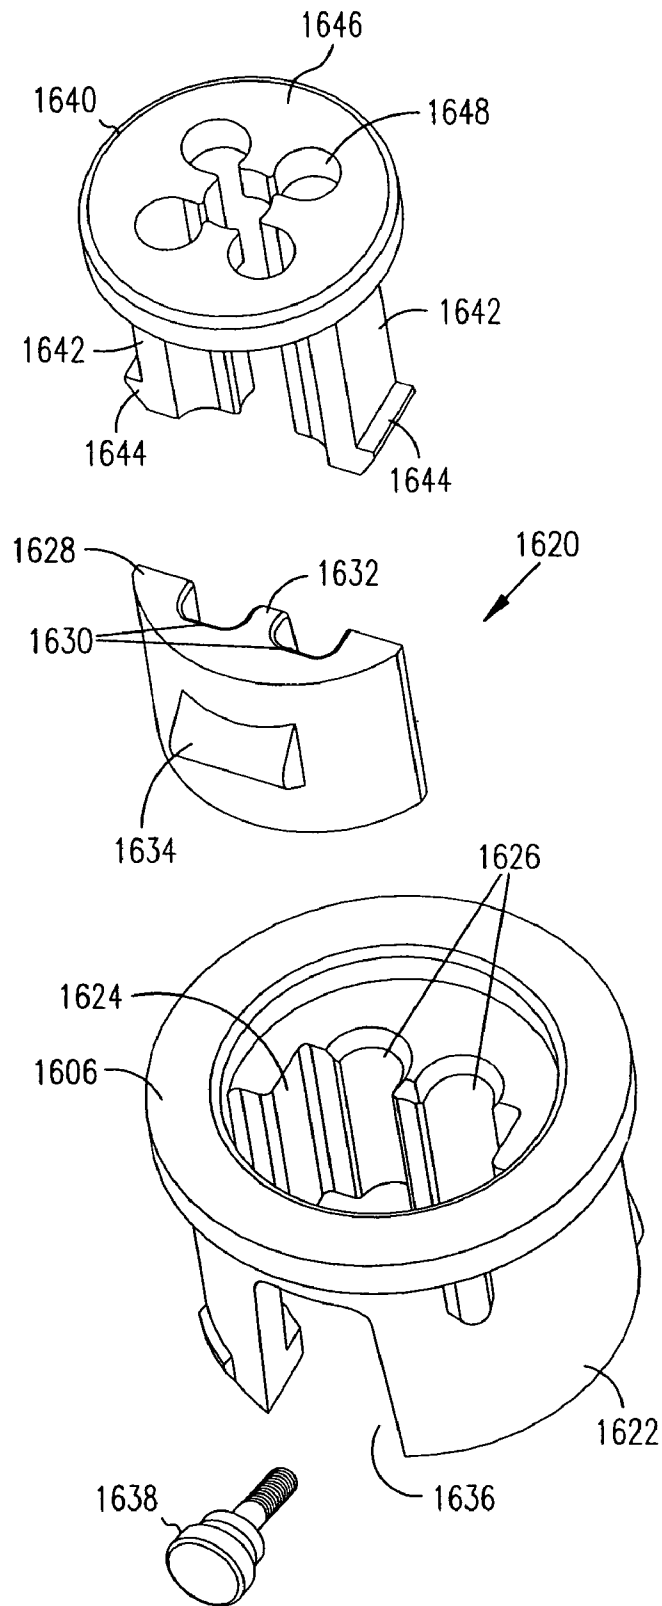


FIG. 16B

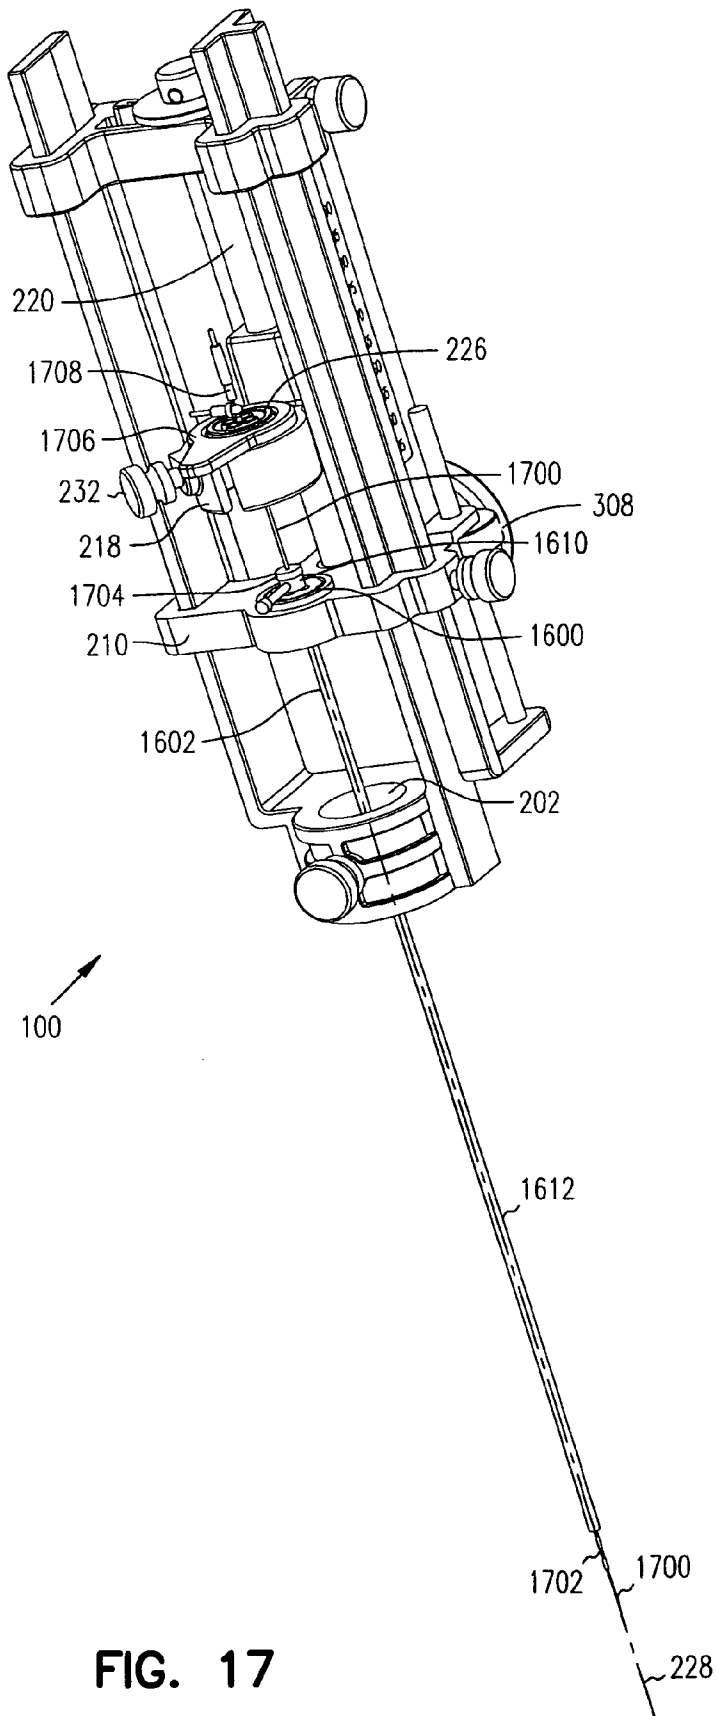


FIG. 17

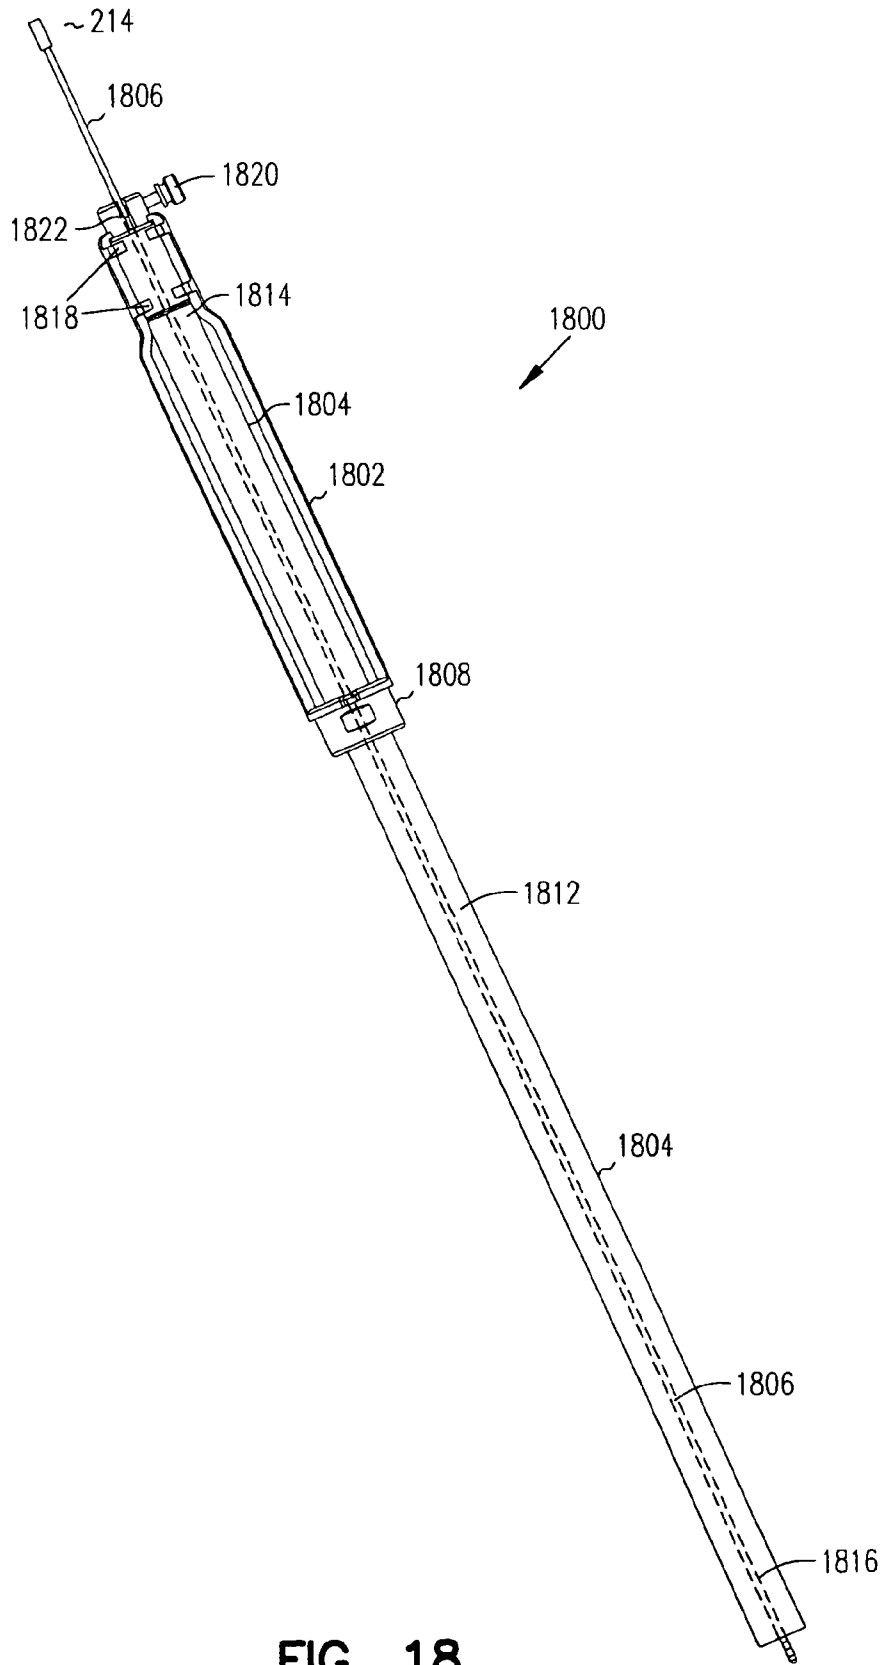


FIG. 18

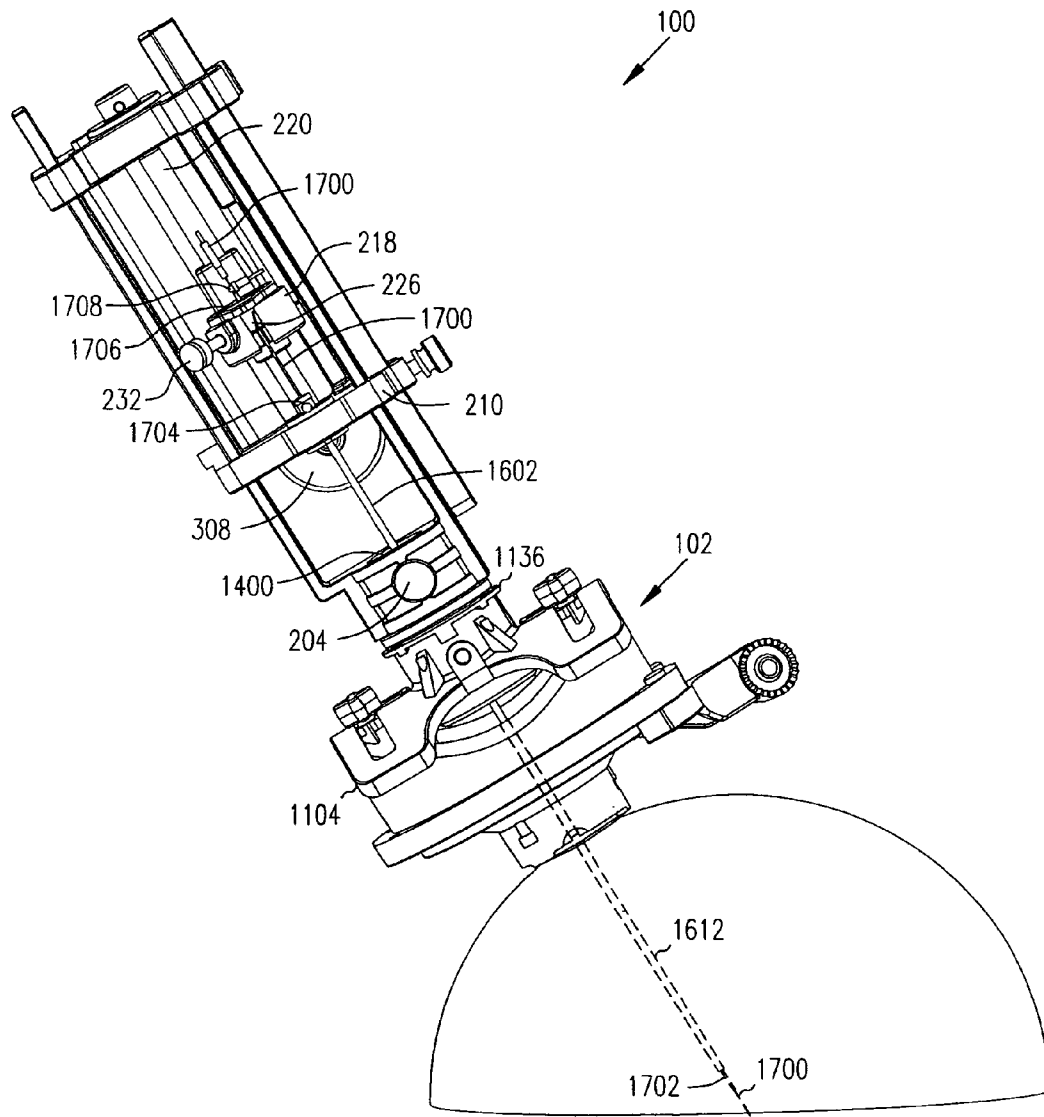


FIG. 19

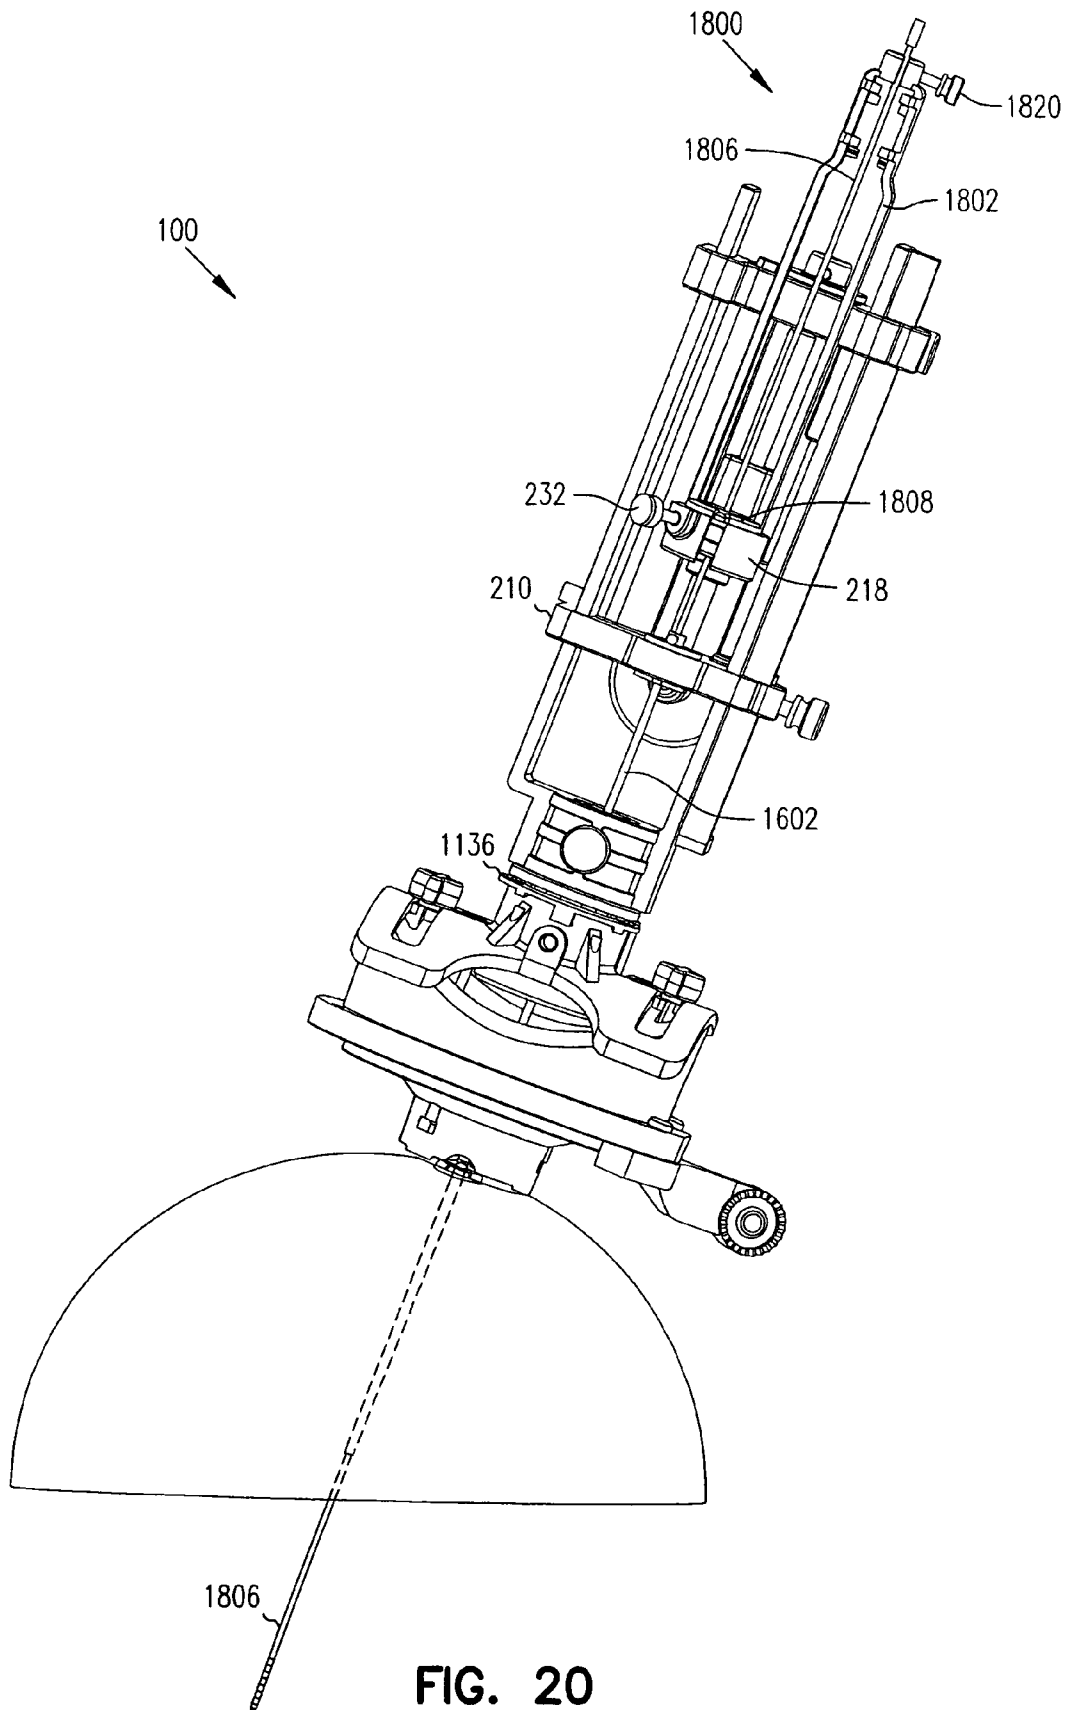


FIG. 20



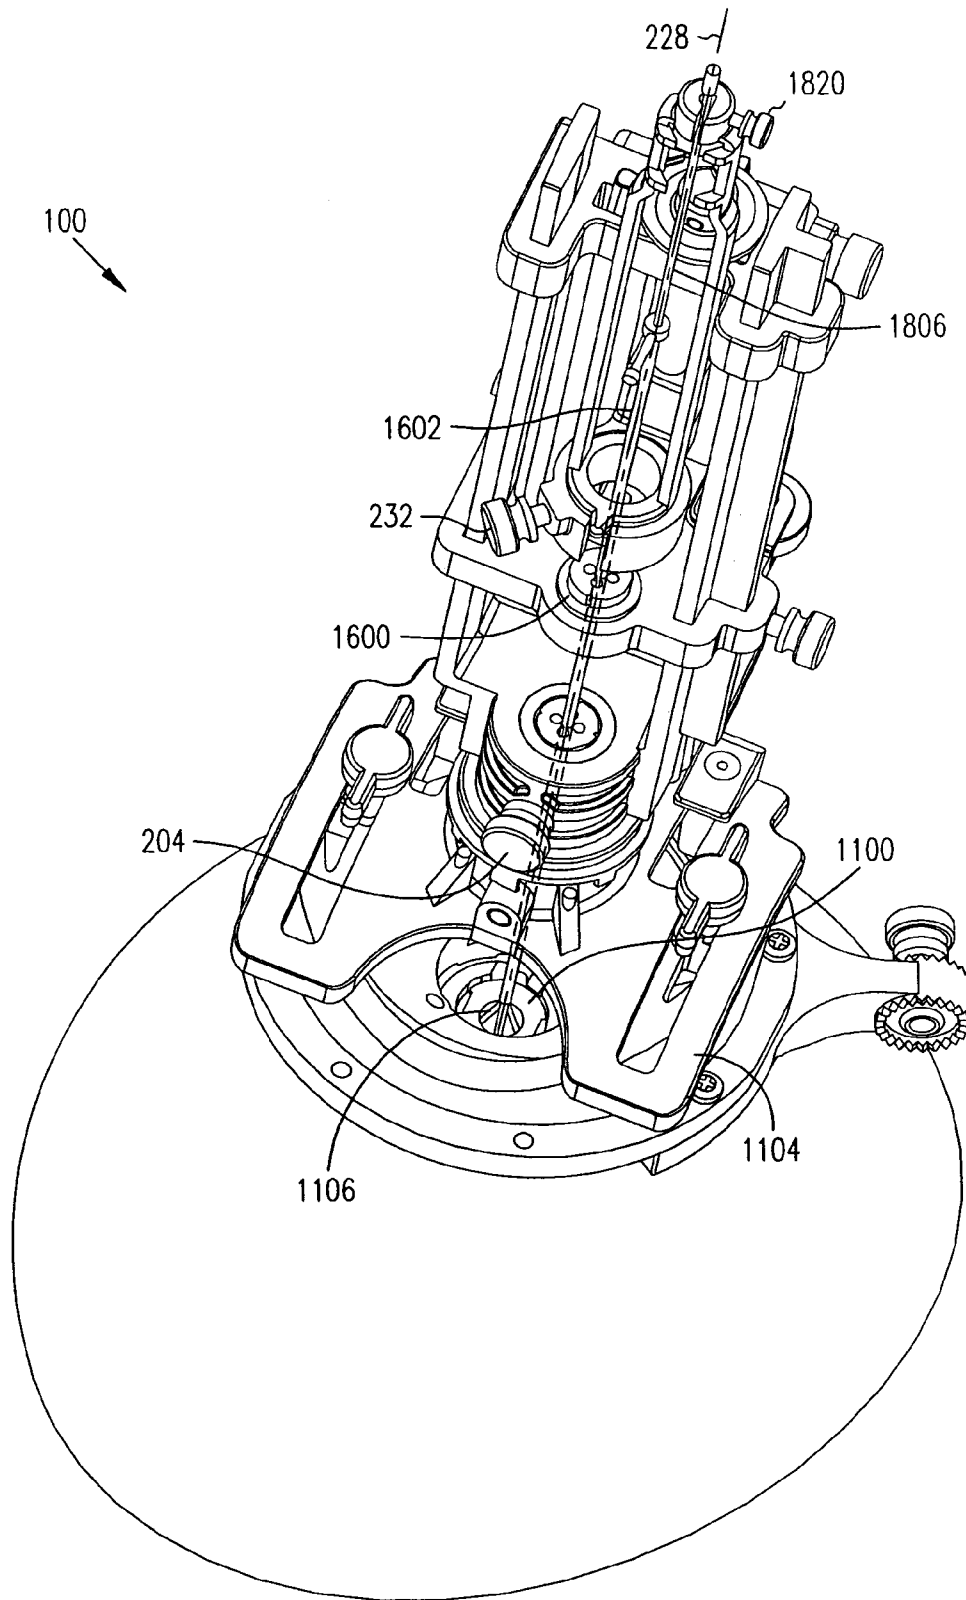


FIG. 21

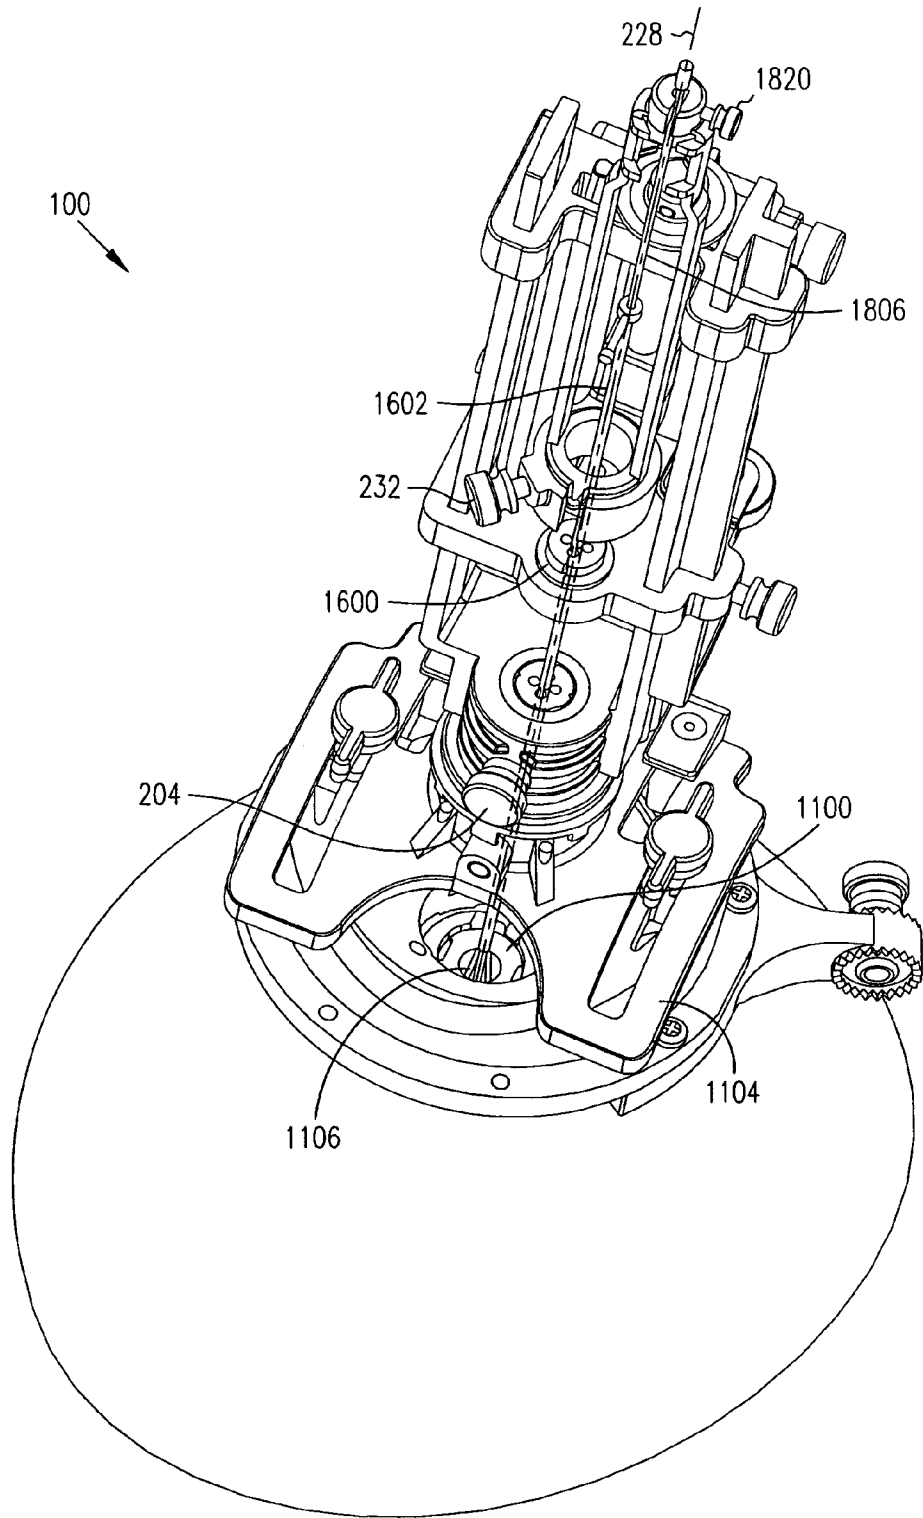


FIG. 22

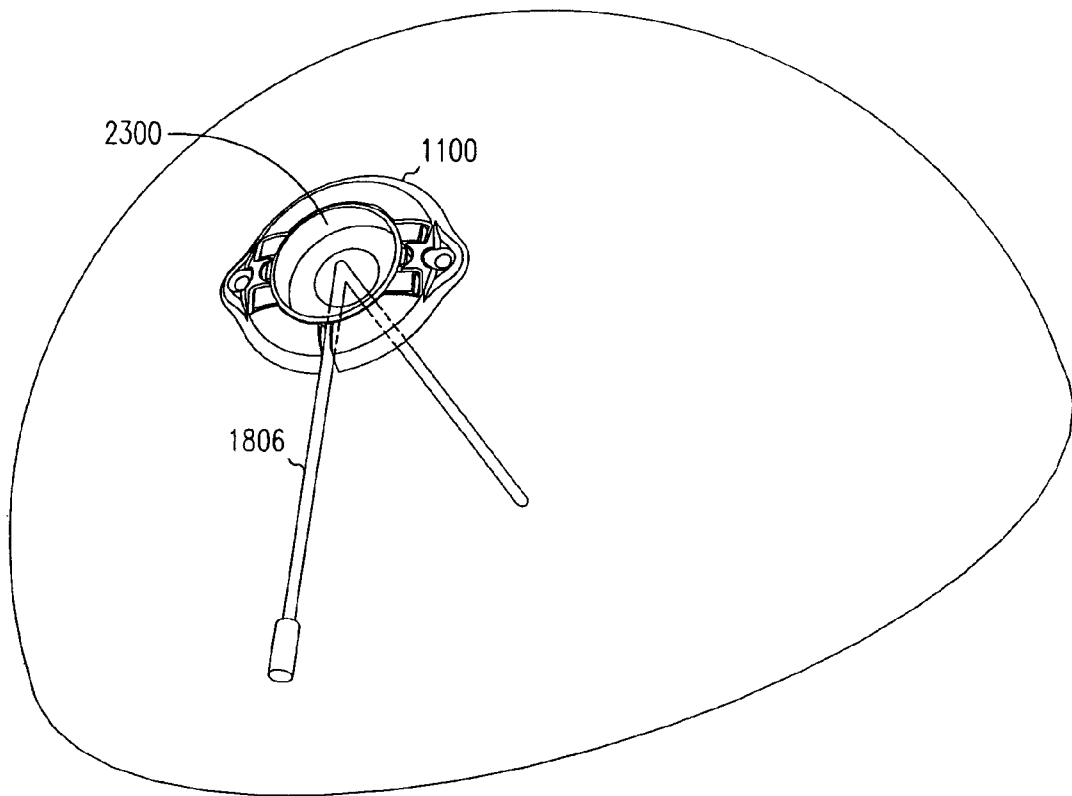


FIG. 23

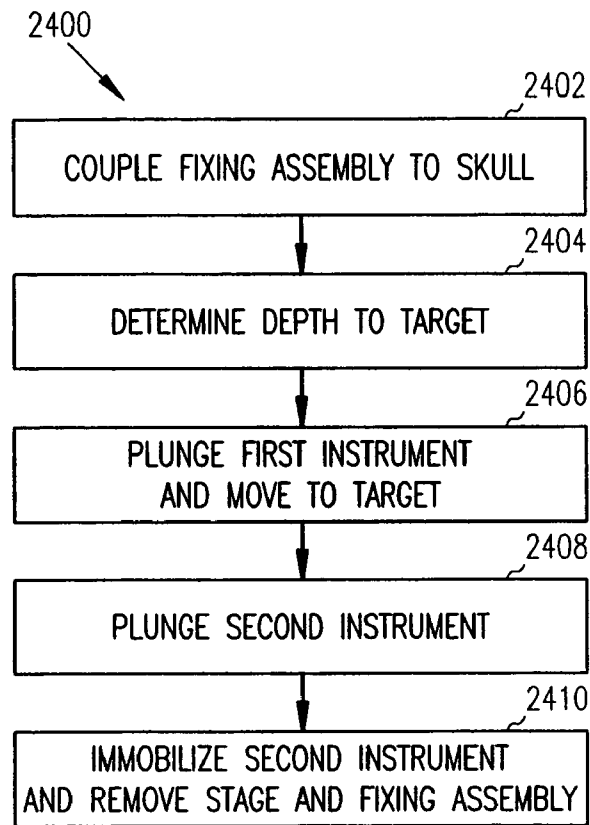


FIG. 24

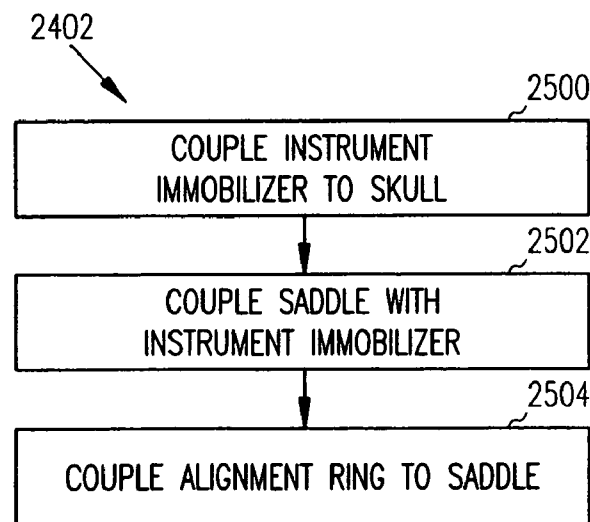


FIG. 25

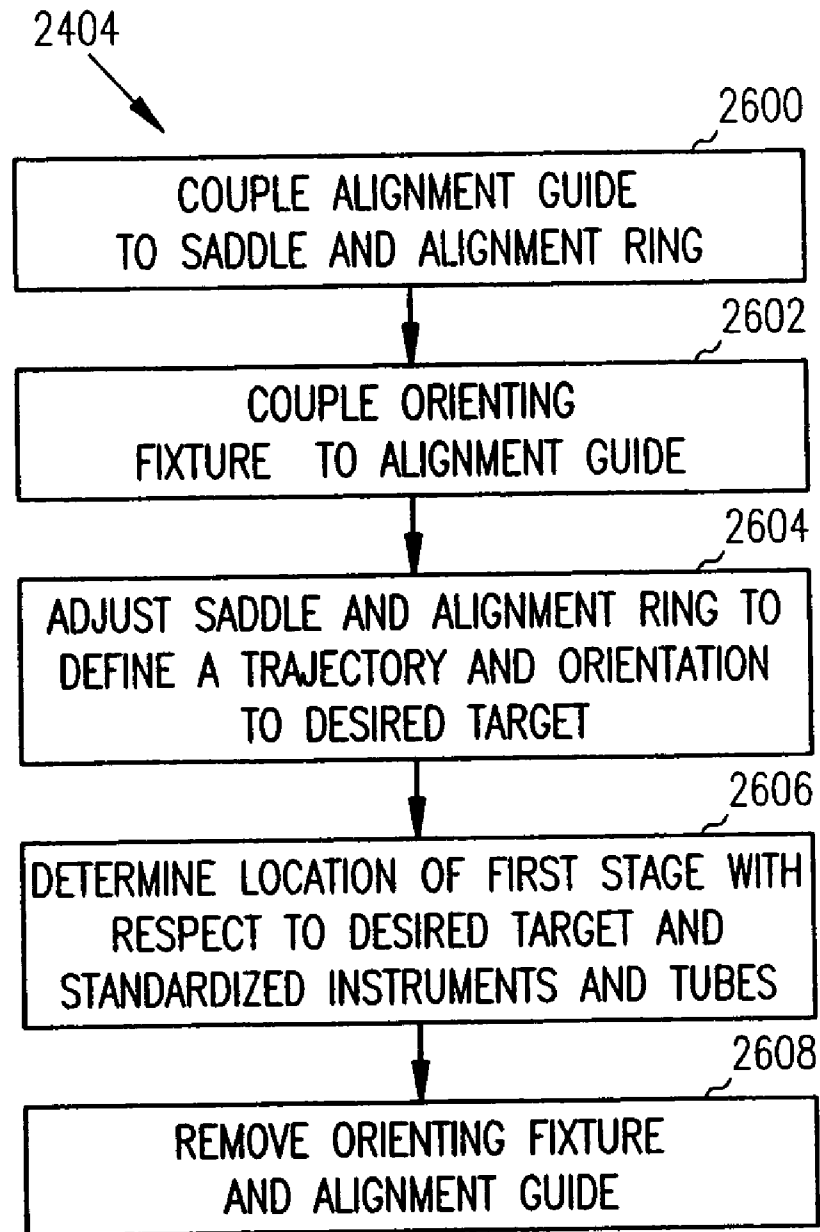


FIG. 26

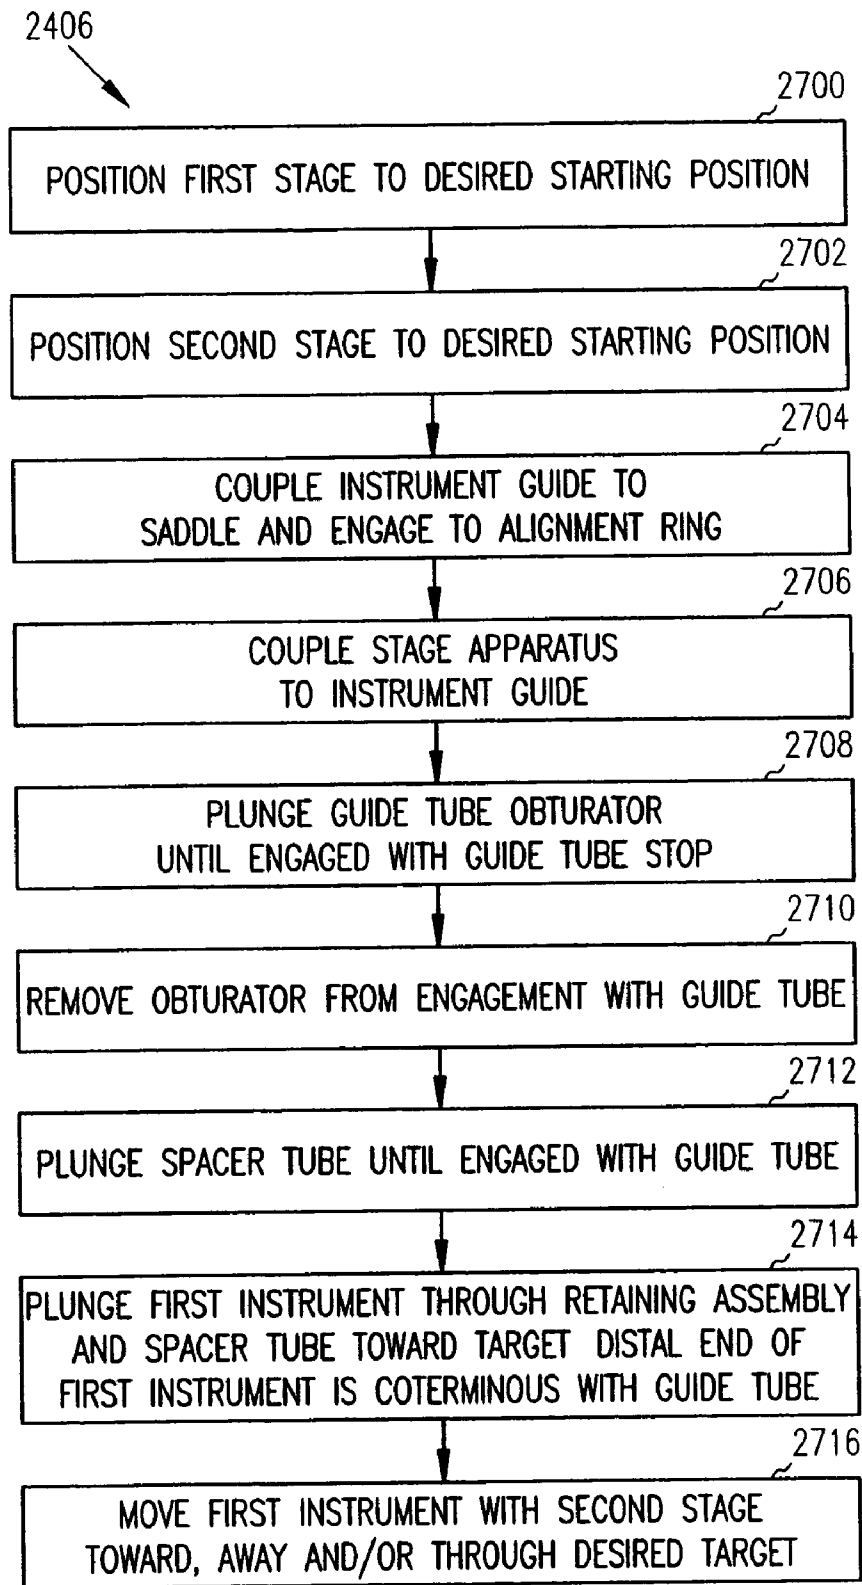


FIG. 27

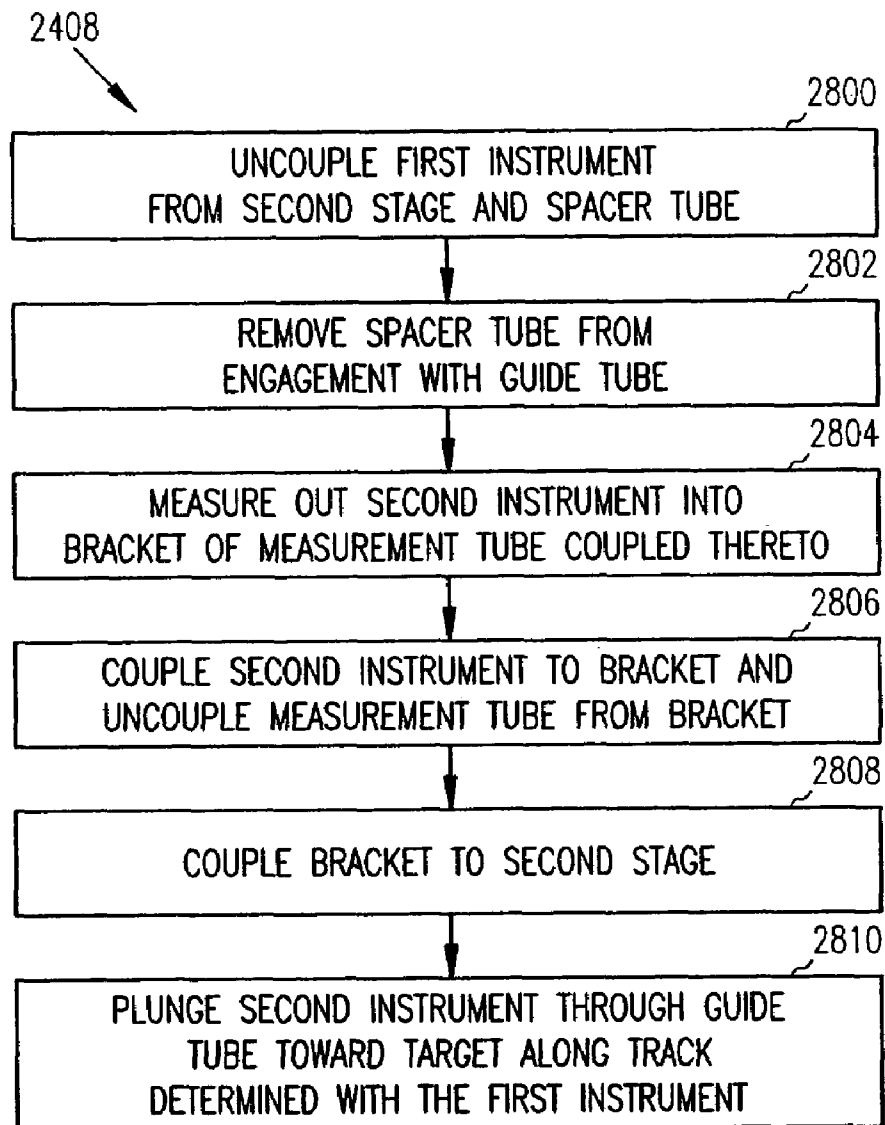


FIG. 28

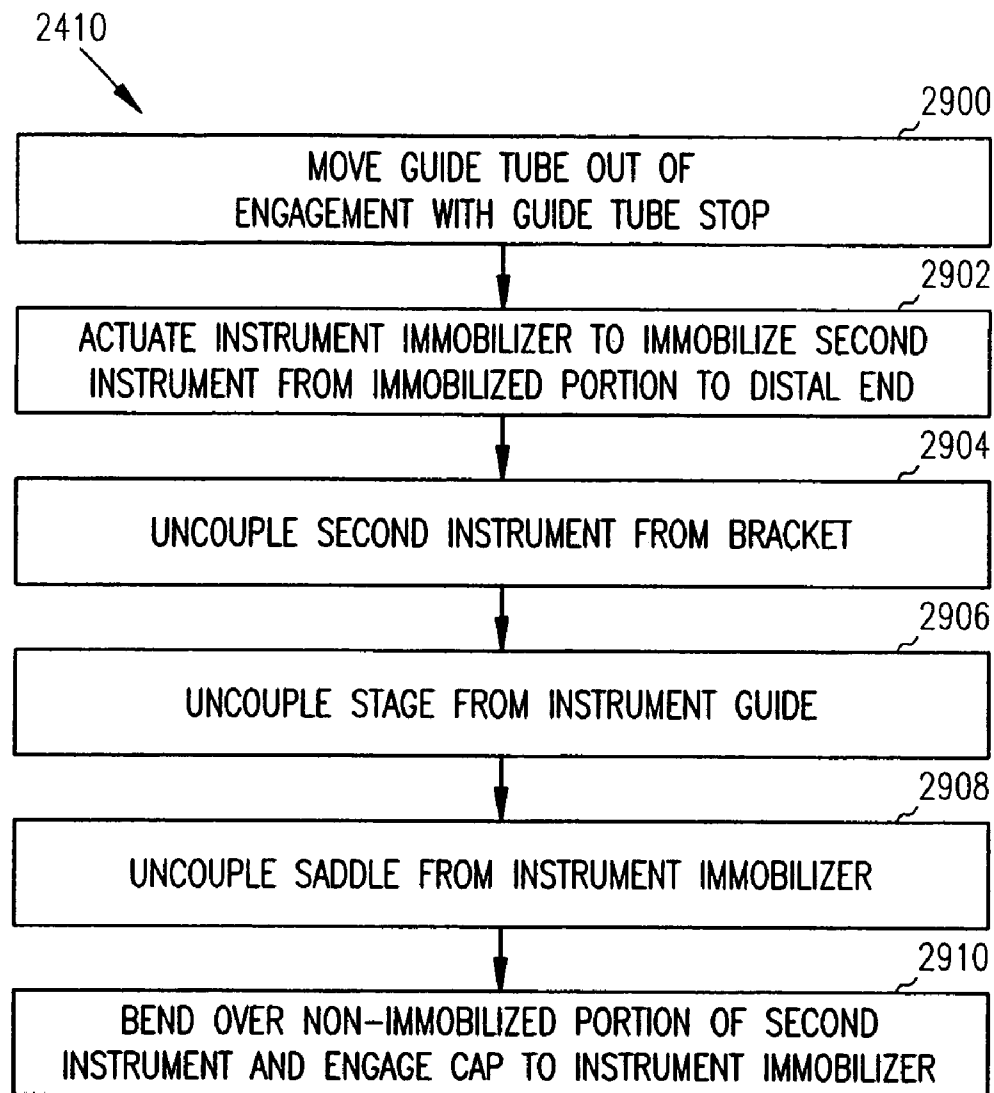


FIG. 29



1

## INSTRUMENT GUIDING STAGE APPARATUS AND METHOD FOR USING SAME

### RELATED APPLICATIONS

This application is related to U.S. patent application Ser. No. 11/005,605, filed on Dec. 4, 2004, entitled "MULTI-LUMEN INSTRUMENT GUIDE," the disclosure of which is incorporated herein by reference in its entirety.

### TECHNICAL FIELD

This document relates generally to a stage from which instruments are positioned and in particular to a stage that provides a known distance from the stage to a target.

### BACKGROUND

Neurosurgery sometimes involves inserting an electrode such as a recording or stimulating electrode (for recording brain signals or providing stimulating pulses), or other instrument (for example, a catheter for fluid aspiration or drug infusion) through a burr hole or other entry portal into a subject's brain towards a target region of the brain. The present inventors have recognized an unmet need for normalizing stage devices, tools, and methods that provide a known distance between a stage and a target, such as to reduce or avoid physician and technician calculations and equipment adjustments.

### BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a perspective view illustrating one embodiment of a normalizing stage and trajectory guide.

FIG. 2 is a perspective view of one embodiment of the normalizing stage.

FIG. 3 is another perspective view of one embodiment of the normalizing stage.

FIG. 4 is a top view of one embodiment of the normalizing stage.

FIG. 5 is a perspective of one embodiment of the normalizing stage.

FIG. 6 is a rear view of another embodiment of the normalizing stage having a potentiometer.

FIG. 7 is a side view of yet another embodiment of the normalizing stage having a hydraulic system.

FIG. 8A is a sectional view of yet another embodiment of the normalizing stage.

FIG. 8B is a sectional view of a further embodiment of the normalizing stage.

FIG. 8C is a perspective view of an embodiment of the first portion of a second stage.

FIG. 8D is a perspective view of one example of a first stage and a second portion of the second stage of the normalizing stage.

FIG. 8E is a perspective view of one example of the first stage and the first portion of the second stage of the normalizing stage.

FIG. 9 is a side view illustrating the fluid inlet and syringe used to fill the hydraulic system, as well as the master cylinder and master piston.

FIG. 10A is a sectional view illustrating an embodiment of a normalizing stage having another hydraulic system.

FIG. 10B is a section view illustrating another example of the fluid inlet and syringe, as well as another example of the master cylinder and master piston.

2

FIG. 11A is an exploded view of a fixture assembly illustrating a skull surface, instrument immobilizer, trajectory guide, and an alignment ring.

FIG. 11B is an exploded view of a fixture assembly illustrating a skull surface, instrument immobilizer, trajectory guide, and another example of an alignment ring.

FIG. 12 is an exploded view of a fixture assembly including the trajectory guide, alignment ring, centered alignment guide, and orienting fixture.

FIG. 13 is an exploded view of a fixture assembly including the trajectory guide, alignment ring, offset alignment guide, and the orienting fixture.

FIG. 14 is a partial section and exploded view of a fixture assembly including the trajectory guide, alignment ring, and centered instrument guide.

FIG. 15 is a partial section and exploded view of a fixture assembly including the trajectory guide, alignment ring, and offset instrument guide.

FIG. 16A is an exploded view showing the normalizing stage, guide tube stop, guide tube, and obturator.

FIG. 16B is an exploded view of the guide tube stop.

FIG. 17 is a perspective view showing the normalizing stage, guide tube stop, guide tube, spacer tube, instrument retaining assembly, and an instrument.

FIG. 18 is a front view of a bracket assembly including the bracket, measurement tube, and an instrument.

FIG. 19 is a perspective view showing the normalizing stage, guide tube stop, guide tube, spacer tube, instrument, instrument guide, trajectory guide, and instrument immobilizer coupled to the skull.

FIG. 20 is a perspective view showing the normalizing stage, guide tube stop, guide tube, bracket, instrument, instrument guide, trajectory guide, and instrument immobilizer coupled to the skull.

FIG. 21 is a perspective view showing the normalizing stage, bracket, instrument guide, instrument immobilizer, trajectory guide, instrument, guide tube stop, and guide tube in an intermediate position.

FIG. 22 is a perspective view showing the normalizing stage, bracket, instrument guide, guide tube stop, guide tube, trajectory guide, instrument, and the instrument immobilizer engaged to the instrument.

FIG. 23 is a perspective view showing the instrument immobilizer, an instrument bent over, and a cap engaged to the instrument immobilizer.

FIG. 24 is a block diagram showing generally an example for using a normalizing stage apparatus and attendant devices.

FIG. 25 is a block diagram showing in more detail an example for coupling a fixing assembly to the skull.

FIG. 26 is a block diagram showing in more detail an example for determining a position of the moveable stage of the normalizing stage apparatus relative to a desired target area.

FIG. 27 is a block diagram showing in more detail an example for plunging and advancing an instrument to the desired target area.

FIG. 28 is a block diagram showing in more detail an example for plunging another instrument to the desired target area.

FIG. 29 is a block diagram showing in more detail an example for immobilizing the other instrument and removing the normalizing stage apparatus and fixing assembly.

## DESCRIPTION OF THE EMBODIMENTS

In the following detailed description, reference is made to the accompanying drawings which form a part hereof, and in which is shown by way of illustration specific embodiments in which the invention may be practiced. These embodiments are described in sufficient detail to enable those skilled in the art to practice the invention, and it is to be understood that the embodiments may be combined, or that other embodiments may be utilized and that structural, logical and electrical changes may be made without departing from the scope of the present invention. The following detailed description is, therefore, not to be taken in a limiting sense, and the scope of the present invention is defined by the appended claims and their equivalents.

In this document, the terms “a” or “an” are used, as is common in patent documents, to include one or more than one. Furthermore, all publications, patents, and patent documents referred to in this document are incorporated by reference herein in their entirety, as though individually incorporated by reference. In the event of inconsistent usages between this document and those documents so incorporated by reference, the usage in the incorporated references(s) should be considered supplementary to that of this document; for irreconcilable inconsistencies, the usage in this document controls.

FIG. 1 is a perspective view illustrating generally a normalizing stage apparatus 100 for positioning an instrument using a stage positioned at a known desired (e.g., predetermined) distance from a target. In one example, the target is a location in a brain. The normalizing stage apparatus 100 is coupled to a patient through a fixture assembly 102, sometimes referred to as a trajectory guide. The fixture assembly 102 is operable to position the normalizing stage 100 in a desired orientation to provide a fixable desired trajectory to the target.

FIG. 2 is a front perspective view of a portion of the normalizing stage 100, which includes a base 200. In this example, an inner surface of the base 200 defines a socket 202, for an instrument guide (described below). A thumb screw 204 or other fixation devices extends through the base 200 and into the socket 202, in this example. The thumb screw 204 is operable to engage an instrument guide and fixedly couple the normalizing stage 100 to the instrument guide. The base 200 further includes guide rails 206A, 206B that extend from a lower portion 208. The longitudinal axis of the socket 202 defines a trajectory 228. The guide rails 206A, 206B are substantially parallel to the trajectory 228 defined by the socket 202. In this example, one of the guide rails 206B has a “T” cross section and the remaining guide rail 206A has an approximately rectangular cross section. In another example, the guide rails 206A, 206B both have approximately rectangular cross sections or other geometries that allow for slidable movement along the guide rails 206A, 206B.

A first stage 210 is coupled to the guide rails 206A, 206B. In this example, the first stage 210 includes a lower portion 222 and upper portion 224. The first stage 210 includes four guide rail lumens, two guide rail lumens 212A, 212B extend through the lower portion 222 and another two guide rail lumens 212C, 212D extend through the upper portion 224. The guide rail lumens 222 are dimensioned and configured to slidably couple with the guide rails 206A, 206B. This enables movement of the first stage 210 along the trajectory 228 defined by the socket 202. Additionally, the span 230 between the upper guide rail lumens 212C, 212D and lower guide rail lumens 212A, 212B aids in preventing unwanted lateral or rotational translation of the stage 210 with respect to the

trajectory 228. In other words, the sliding relationship of the guide rails 206A, 206B to the guide rail lumens 212A, B, C, D of the first stage 210 constrains lateral movement of the first stage with respect to the trajectory 228, while allowing movement along the trajectory. A thumb screw 214 or other fixation device extends through a portion of the first stage 210 and into the guide rail lumens 212B. The thumb screw 214 is operable to engage one of the guide rails 206A, 206B and immobilize the first stage with respect to the base 200. The first stage 210 also includes a lumen 216. The lumen 216 is substantially aligned with the socket 202. When the first stage 210 is advanced along the trajectory 228 the lumen 216 remains aligned with the trajectory 228.

FIG. 3 is a rear perspective view of the same portion of the normalizing stage 100 including three scales 316A-C. A first stage actuator 300, comprising a knob in this example, is coupled to the first stage 210. In this example, a stationary screw 302 is coupled to the base 200. In this embodiment, the stationary screw 302 extends through and is coupled to the first stage actuator 300. The stationary screw 302 is also coupled to the first stage 210. In this example, the stationary screw 302 is substantially parallel to the trajectory 228 (FIG. 2). The first stage actuator 300 is operable to advance the first stage 210 along the trajectory 228 by rotating the actuator 300. The first stage actuator 300 includes threads on an inner surface which engage corresponding threads of the stationary screw 302. The stationary screw 302 is long enough to enable a desired position of the first stage 210 with respect to the desired target of substantially all subjects into which an instrument is to be introduced.

In this embodiment a scale 304 is provided, such as along a side of the first stage 210 near a guide rail 206B. The scale 304 is graduated to indicate a range of positions of the first stage 210 with respect to a desired target. A reference mark 306 on a guide rail 206B is positioned to cooperatively indicate, with the graduated scale 304 on the first stage 210, the position of the first stage with respect to the target.

Referring again to FIG. 2, a second stage 218 is movably coupled to the first stage 210. In one example, the second stage 218 is coupled to the first stage 210 by a screw 220 or the like. The screw 220 extends between the lower portion 222 and upper portion 224 of the first stage 210 and is rotatably coupled to each. The second stage 220 includes a lumen having inner threads engaging the threads for screw 220. Additionally, the second stage 218 includes a retaining assembly orifice 226 dimensioned and configured to couple with a retaining assembly, as described below. In this example, the retaining assembly orifice 226 is a broken ring. In another example, the retaining assembly orifice 226 is defined by a continuous inner surface of the second stage 218. A thumb screw 232 or other fixation device is coupled to and extends through a portion of the second stage 218. The thumb screw 232 is operable to immobilize an instrument extending through the retaining assembly lumen 226.

FIG. 3 is a perspective view of the normalizing stage 100. As shown in the example illustrated in FIG. 3, an actuator knob 308 is coupled to the first stage 210. The actuator knob 308 is connected by cooperative gearing to the screw 220 (FIG. 2), in this example. The knob 308 is thus operable to move the second stage 218 along the screw 220. Additionally in this example, the second stage 218 includes a protrusion 310 which extends from a surface of the second stage through a slot 312 in the first stage 210. The protrusion 310 maintains the alignment of the second stage 218 to the first stage 210 during rotation of the knob 308, which turns the screw 220.

Specifically, the slot **312** helps the retaining assembly orifice **226** to remain aligned with the guide tube stop lumen **216** and instrument guide lumen **202**.

In the example shown in FIG. 3, the protrusion **310** also includes a reference marking **314**. The reference marking **314** indicates the position of an instrument with respect to the standardized distance to target. In one example, a scale **316A-C** is included on the first stage **210**. The scale **316A-C** is disposed adjacent to the slot **312**. In one example, the reference marking **314** is read against the scale **316A** to determine the position of the instrument with respect to the target. Optionally, the scale **316A** and marking **314** show the position of a tip of the instrument with respect to the target. In another example, scale **316B** is included on the first stage **210** in place of scale **316A**. Scale **316B** in cooperation with the marking **314** has the "0" of the scale **316B** corresponding to the top of the travel of the second stage **218**. Scale **316C**, in yet another example, cooperates with marking **314** so the "0" of the scale **316C** corresponds to an approach distance remote from the desired target. As a result, when the mark **314** is located at the "0" of the scale **316C** the tip of the instrument is positioned a desired (e.g., predetermined) approach distance (e.g. 15 millimeters) from the desired target. In still another example, the scales **316A-C** are adjustable (for example, removable and reattachable, such as with an adhesive backing) and is positioned along the slot **312** according to the needs of the physician or technician. The mark **314** is part of a vernier scale **318**, in another option, and the vernier scale **318** provides another degree of precision for measuring the distance from the instrument to the desired target.

FIG. 4 is a top view of one embodiment of the normalizing stage **100**. A circular fine scale **400** is coupled to the top of the screw **220**. The screw **220** is threaded. Each rotation of the screw **220** correspond to one rotation of the fine scale **400**. In one example, one rotation of the screw **220** moves the second stage **218** by 1 mm toward or away from the target. In this example, the fine scale **400** is graduated so one rotation of the scale indicates 1 mm of advancement, and 0.1 mm and 0.01 mm increments are also indicated. A reference marking **402** is included on the first stage **210** to indicate the position of the second stage **218** when reading the fine scale **400**. The scale **400**, in one option, includes an inner scale **404** and an outer scale **406**. The inner scale **404** is used to measure translation of the second stage **218** from the "0" marking on scale **316A**, **316C** to a measure above "0" in another option (e.g. from 10.6 millimeters to 10.7 millimeters above "0"). In yet another option, the outer scale **406** is used to measure translation of the second stage **218** from the "0" marking on the scale **316A**, **316C** to a measure below "0", for instance from 4.0 millimeters to 4.1 millimeters below "0." As a result, the inner scale **404** is used to measure translation of the second stage **218** above "0" and the outer scale **406** is used to measure translation of the second stage **218** below "0."

FIG. 5 is a bottom perspective view of one embodiment of the normalizing stage **100**. The socket **202** includes keyed slots **500** or the like within the base **200**. When the normalizing stage **100** is coupled to an instrument guide (described below), the surfaces defining the keyed slots **500** engage corresponding keys present on the instrument guide. Unwanted rotation of the normalizing stage **100** is thus prevented with respect to the instrument guide.

FIG. 6 is a rear view of another embodiment of the normalizing stage **100**. In this embodiment, the position of the second stage **218** with respect to the first stage **210** is measured by a potentiometer assembly **600**. The assembly **600** includes a wiper **602**. In this example, the wiper **602** is coupled to the second stage **218**. Alternatively, the wiper **602** is coupled to

the first stage **210**. The wiper **602** electrically contacts and bridges between two elongate resistors **604** physically parallel to one another and coupled to the first stage **210**. The resistors **604** are of sufficient length to enable the second stage **218** to advance an instrument toward, away, and/or through a target while still contacting the wiper **602** to measure the position of the second stage **218**. In one example, a cable **606** connects the potentiometer assembly **600** to an output device that includes a display screen. The output device displays the location of the second stage **218** according to the position of the wiper **602** with respect to the resistors **604**. In another example, the output device displays the location of an instrument with respect to a desired target in a similar manner as with the scales **316A-C** (described above). In an alternate example, the resistors **604** are coupled to the second stage **218** and the wiper **602** is coupled to the first stage **210**. In another option, supplemental resistors are coupled to the base **200** or the first stage **210** and a supplemental wiper is coupled to the other of the base **200** or the first stage **210**. As a result, a potentiometer assembly is used to measure translation of the first stage **210** with respect to the base **200**.

FIG. 7 illustrates a side view of another embodiment of the normalizing stage **100** that includes a hydraulic system **700**. The hydraulic system **700** includes, in fluid communication with each other, a hydraulic cylinder **702**, hydraulic piston **704**, master hydraulic cylinder **706**, and master hydraulic piston **708**. The master hydraulic cylinder **706** and piston **708** are operable to actuate the hydraulic cylinder **702** and piston **704**. In one example, the hydraulic cylinder **702** and piston **704** move the second stage **218** with respect to the first stage **210**.

FIG. 8A is a cross section view of the hydraulic embodiment of the normalizing stage **100**. In this example, the hydraulic cylinder **702** is mounted to the first stage **210** and the hydraulic piston **704** is mounted to the second stage **218** (or vice versa). In this example, the hydraulic piston **704** is coupled to the second stage **218** by a piston tube **800**. In one example, a hydraulic line **802** coupled to the master piston **708** (FIG. 7) extends through the piston tube **800** and is coupled substantially adjacent to the hydraulic piston **704**. In another example, the hydraulic line **802** is coupled to the piston tube **800** at any location along the length of the piston tube **800**. In yet another example, the hydraulic line **802** is coupled to the second stage **218** and in fluid communication through a coupling to the piston tube **800**. The inner surface of the hydraulic cylinder **702** and hydraulic piston **704** define a first volume **804**. The first volume **804** is increased and decreased by actuation of the master cylinder **706** and master piston **708**. Changing the first volume **804** advances the piston **704** inside the cylinder **702**, which, in turn, advances the second stage **218**.

In the example shown in FIG. 8A, a spring housing **806** is coupled to the first stage **210**. In this example, the housing **806** is a tubular structure. A spring **808** or the like is coupled to one end of the housing **806**, in one example. The other end of the spring **808** is coupled to the second stage **218**. In another example, an elastic material, for example an elastomeric membrane is coupled between the housing **806** and the second stage **218**. The spring **808** is in tension and maintains a force on the second stage **218**. In other words, the spring **808** pulls the second stage **218** and the hydraulic piston **704** toward the fluid filled end of the hydraulic cylinder **702**. The incompressibility of hydraulic fluid in the hydraulic cylinder **702** prevents the spring **808** from undesirably advancing the second stage **218**. The spring **808** thus maintains a pressurized hydraulic system **700** by pulling the piston **704** toward

the cylinder **702**. In this example a stopcock valve **810** or the like is coupled to the hydraulic cylinder **702** and is in fluid communication thereto.

The second stage **218**, shown in FIG. **8A**, is slidably mounted on and guided by a guide rail **812** associated with the first stage **210**. Guide surface **814** of the second stage **218** provides smooth linear motion of second stage **218** along an interface **816** with the guide rail **812**. Guide surface **814**, in one example is integral with the second stage **218** (FIG. **8A**). In another example, guide surface **814** includes a friction-reducing insert or coating made of a bearing material, including but not limited to, TEFLON. Optionally, the coating or insert is coupled along the guide rail **812**.

Another example of the normalizing stage **100** is shown in FIG. **8B**. The second stage **218** includes at least one recirculating bearing **818** including ball bearings **820**. The recirculating bearing **818** is at the interface **816** between the second stage **218** and guide rail **812** and thereby reduces friction first and second stages **210**, **218**. As shown in FIG. **8B**, the recirculating bearing is a linear bearing to permit linear movement along the guide rail **812**. In another example, the bearing **818** is a conventional non-circulating type. In yet another example, the recirculating bearing **818** is a flat bearing that rides along the guide rail **812**. The guide rail **812** includes at least one groove **822** for receiving the ball bearings **820** of the flat recirculating bearing **818** to align the second stage **218** and thereby prevent undesired rotation of the second stage **218** around the guide rail **812**. In still another example, the recirculating bearing **818** is a round bearing having a circular inner perimeter at the interface **816**. Optionally, the second stage **218** includes a pair of round recirculating bearings **818** that ride on dual guide rails **812** to prevent undesired rotation of the second stage **218**. The bearings **818** substantially reduce friction at the interface **816** thereby facilitating increased responsiveness of the second stage to actuation with the hydraulic actuator (e.g., the master hydraulic cylinder **706** and the master hydraulic piston **708**).

In another example, a gas vent **824** is substituted for the valve **810**. The gas vent **824** is coupled to the hydraulic cylinder **702** and in fluid communication thereto. When the hydraulic system **700** is filled (as described below) hydraulic fluid fills the volumes defined by the cylinders **702**, **706**, pistons **704**, **708** and the hydraulic line **802**. The air or other gas present in these spaces is forced out by introduction of the fluid. The valve **810** or gas vent **824** permits the gases to escape from the hydraulic system **700**, but retains the hydraulic fluid therein. While gas permeable, the gas vent **824** is not liquid permeable. In one example, the gas vent **824** is a membrane comprised of polytetrafluoroethylene sold under the trademark TEFLON. In another example, any liquid impermeable membrane that otherwise is gas permeable is used as the gas vent **824**.

FIGS. **8C-E** illustrate another example of bearings coupled between the first stage **210** and the second stage **218**. One example of a first portion **825** of the second stage **218** including three rollers **826** (e.g., needle rollers) is shown in FIG. **8C**. In another example, the second stage **218** includes one or more rollers **826** (e.g., eight needle rollers). The rollers **826** are coupled to the first portion **825** with axles **827** that permit rotation of the rollers **826**. The axles **827** have a small diameter to decrease bearing friction between the rollers **826** and the first portion **825**. The first portion **825** of the second stage **218** shown in FIG. **8C** is sized and shaped to couple along one side of the guide rails **812** (FIGS. **8D, E**). Optionally, as shown in FIG. **8D**, a second portion **828** of the second stage **218** having rollers **826** (FIG. **8E**) is sized and shaped to couple along an opposed side of the guide rails **812** relative to the first

portion **825**. The first and second portions **825**, **828** are coupled together, in one example, with fasteners **830** (FIG. **8D, E**) such as screws, rivets, mechanical fittings and the like.

FIGS. **8C-E** show one example of how the rollers **826** are arranged around the guide rails **812** to permit linear movement of the second stage **218** with substantially reduced friction. As shown in FIGS. **8D, E** the guide rails **812** are sized and shaped to contact the rollers **826** of the first and second portion **825**, **828** at angles intended to limit the movement of the second stage **218** to linear movement along the guide rails **812**. The first and second portions **825**, **828** of the second stage **218** are correspondingly sized and shaped to position the rollers **826** along the angled surfaces of the guide rails **812**. Importantly, the arrangement of the rollers **826** allows linear movement of the second stage **218**, but otherwise prevents unwanted rotation of the second stage **218** around the guide rails **812**. In another example, the guide rails **812** and the first and second portions **825**, **828** are sized and shaped in a variety of orientations that cooperate to permit linear movement of the second stage **218** without allowing rotation around the guide rails **812**. For example, four rollers are positioned at angles relative to each other around a guide rail. Optionally, additional rollers are provided to enhance reduction of friction while allowing linear movement of the second stage **218** relative to the first stage **210**.

FIG. **9** is a side view illustrating a fluid inlet **900** and syringe **902** used to fill the hydraulic system **700**. In this example, the fluid inlet **900** is coupled to the master hydraulic cylinder **706** and is in fluid communication thereto through a manifold **908** that includes a portion of the hydraulic line **802**, which is also in fluid communication with the master hydraulic cylinder **706**. In another example, the fluid inlet **900** is in direct fluid communication with the master hydraulic cylinder **706**. The fluid inlet **900** includes a socket **904** and check valve **906**. The check valve **906** prevents fluid introduced at the inlet **900** from leaking out at the inlet **900**. In the example shown in FIG. **9**, a stopcock **912** is coupled to the check valve **906** and in fluid communication thereto. The syringe **902** includes a nozzle **910** dimensioned and configured to snugly couple with the socket **904** of the fluid inlet **900**. The syringe **902** is filled with a hydraulic fluid (for example, sterile saline) and the nozzle **910** is inserted into and coupled to the socket **904**. The plunger **915** of the syringe **902** is then depressed. This forces the hydraulic fluid from the syringe **902** into the fluid inlet **900** and hydraulic system **700**. In one example, the syringe **902** injects enough hydraulic fluid into the system **700** to fill the volume defined by the cylinders **702**, **706**, pistons **704**, **708**, and hydraulic line **802** and allow a full range of movement for the second stage **218**. In another example, the syringe **902** is filled and used multiple times to fully fill the hydraulic system **700**.

The master hydraulic cylinder **706** and master hydraulic piston **708** are shown in FIG. **9**. As described above, the master hydraulic piston **708** is coupled to the master hydraulic cylinder **706** to allow slidable movement therebetween. The inner surface of the master cylinder **706** and the master piston **708** define a second volume **914**. The second volume is increased and decreased by actuation of a screw **916**, a distal end of which is coupled to the master piston **708** and the master cylinder **706**. The threaded outer surface of the screw **916** engages a correspondingly threaded inner surface of the master cylinder **706**. Rotation of the screw **916** advances the screw, and thus the master piston **708**, with respect to the master cylinder **706**. A knob **918** is coupled to a proximal end of the screw **916** to enable rotation of the screw. Changing the second volume **914** correspondingly changes the first volume **804** in a substantially inverse manner by moving hydraulic

fluid through the hydraulic line 802. In other words, decreasing the second volume 914 similarly increases the first volume 804, and increasing the second volume decreases the first volume in substantially the same way. The screw 916 thus operates to move the second stage 218 through actuation of the master cylinder 706, master piston 708, hydraulic cylinder 702, and hydraulic piston 704.

FIG. 10A is a sectional view of another embodiment of normalizing stage 100 including a rolling diaphragm hydraulic system 1000. In this example, hydraulic system 1000 includes a piston 1002 disposed within a cylinder 1004. In one example, a flexible fluid impermeable membrane 1006 extends from a surface defining the circumference of piston 1002. The membrane 1006 is coupled to the cylinder 1004. The membrane 1006, piston 1002, and cylinder 1004 define a first volume 1008. The first volume 1008 is changed by actuation of the master piston 708 and master cylinder 706 via screw 916 (described above). The flexible membrane 1006 provides a seal between the cylinder 1004 and piston 1002 while one piece moves with respect to the other. In an example, there is sufficient clearance between the cylinder 1004 and piston 1002 for the flexible membrane to fold between the cylinder and piston. In other words, the cylinder 1004 and piston 1002 move without directly contacting one another. Expanding and contracting the first volume 1008 thereby produces substantially little friction between cylinder 1004 and piston 1002. Thus, more accurate and responsive movement of the piston 1002 with respect to the cylinder 1004 is possible.

In one example, a spring 1014 or the like is disposed between piston 1002 and cylinder 1004. The spring 1014 is optionally in compression and maintains a force on the piston 1002 relative to the cylinder 1004. The spring 1014 pushes piston 1002 and, with it, second stage 218 toward the fluid filled end of the cylinder 1004. The incompressibility of hydraulic fluid in the cylinder 1002 prevents the spring 1014 from undesirably moving the second stage 218. The spring 1014 thus maintains a pressurized hydraulic system 1000 by pushing the piston 1002 toward the cylinder 1004.

Referring now FIG. 10B, in another example, a flexible liquid impermeable membrane 1018 for a rolling diaphragm extends between the master hydraulic cylinder 706 and master hydraulic piston 708. The master hydraulic piston 708 is coupled to master hydraulic cylinder 706 with a rolling diaphragm similarly to how piston 1002 and cylinder 1004 are coupled in FIG. 10. The rolling diaphragm provided with the flexible membrane 1018 facilitates enhanced movement of the piston 708 relative to the cylinder 706 by reducing friction therebetween. Additionally, the reduced friction provided by the flexible membrane 1018 improves responsiveness between rotation of the knob 918 and movement of the piston 708 thereby enhancing overall responsiveness at the piston 1002 and the cylinder 1004 of the normalizing stage 100 (FIG. 10).

In yet another example shown in FIG. 10B, the syringe 902 and stopcock 912 couple to hydraulic line 802 between hydraulic system 1000 and the master hydraulic system 700. Coupling the fluid inlet 900 provided by the syringe 902 and the stopcock 912 along the line 802 eliminates the need for the manifold 908 (FIG. 9). Additionally, the fluid inlet 900 is in closer communication with the hydraulic system 1000 facilitating easier filling of the system 1000.

An inlet 1010 to the first volume 1008 is provided through the cylinder 1004. The inlet 1010 and the first volume 1008 are in fluid communication with the hydraulic line 802. A

stopcock valve 1012 is coupled to the cylinder 1004 and is operable to open or seal the system 1000 for hydraulic fluid filling.

As described in a previous example, a gas vent can be substituted for stopcock valve 1012 in FIG. 10. In this example, as before, air or other gas in first volume 1008 escapes through the gas permeable membrane of the vent. In one example, end surface 1016 of cylinder 1004 is replaced with a suitably-supported gas permeable membrane. Because hydraulic system 1000 is under pressure relative to the surrounding atmosphere (e.g., due to spring 1014), gas or air bubbles are forced out of the hydraulic fluid when they contact the surface of the membrane. The large surface area and direct path at the end surface 1016 facilitate the escape of gas or air from within the hydraulic system 1000. In this way, hydraulic system 1000 easily fills completely with incompressible hydraulic fluid (e.g., sterile saline). In another example, both hydraulic system 1000 and the master hydraulic system 700 include gas vents as just described.

The position of the second stage 218 relative to the first stage 210, in one example including the hydraulic systems 700, 1000, is measured with a potentiometer, such as potentiometer assembly 600 (described above). The potentiometer assembly 600 provides accurate and precise indications of the second stage 218 position with respect to the first stage 210. In another example, the potentiometer assembly 600 indicates the position of an instrument with respect to the desired target (as described above). The potentiometer assembly 600 allows for direct measurement of movement of the second stage 218 relative to the first stage 210. The potentiometer assembly 600 overcomes measurement error due to lag or hysteresis caused by deformability of the materials used in the hydraulic systems 700, 1000. Measurement error typically appears when measuring the position of the hydraulic pistons 704, 1002 relative to the hydraulic cylinders 702, 1002 by translation of the master piston 708 relative to the master cylinder 706. The potentiometer assembly 600 also overcomes measurement error caused by friction in the hydraulic systems 700, 1000, for instance between the hydraulic cylinders 702, 706, 1004 and hydraulic pistons 704, 708, 1002. Measurement error is overcome by directly measuring the translation of the second stage 218 relative to the first stage 210 with the potentiometer assembly 600.

FIG. 11A is an exploded view of a portion of the fixture assembly 102. An instrument immobilizer 1100 is coupled to the surface of a skull 1102 around a burr hole in the skull 1102. In this example, the instrument immobilizer 1100 is coupled to the surface of the skull 1102 by bone screws extending through the immobilizer and into the skull. The immobilizer 1100 further includes a retaining piece 1106. The retaining piece 1106 is operable to engage and immobilize a portion of an instrument (described below). Additional examples of instrument immobilizers are shown in PCT Patent Application No. PCT/US03/28966 filed on Sep. 17, 2003, which is assigned to the assignee of the present patent application, and which is incorporated by reference herein in its entirety.

Additionally, in this example, a saddle assembly 1104 is coupled to the instrument immobilizer 1100 and aligned with an orthogonal 1134 axis through a center of the instrument immobilizer 1100. Specifically, a base ring 1108 is coupled to the instrument immobilizer 1100. In one example, the saddle assembly 1104 is initially aligned with the orthogonal axis 1134, but coupled to the skull surface 1102. The orthogonal axis 1134 is substantially orthogonal to the surface of the skull 1102. The saddle assembly 1104 further includes a cylindrical sectional tower base 1110 that is dimensioned and

## 11

configured to couple with the base ring 1108 to allow rotation therebetween. A saddle slide 1112 is coupled to the tower base 1110. Thumbscrews 1114 or the like extend through slots 1116 of the saddle slide 1112 and the tower base 1110. The thumbscrews 1114 engage blocks 1118 disposed adjacent to the base ring 1108. The blocks 1118 engage a lip of the base ring 1108. The saddle slide 1112 is operable to move in an arcuate motion with respect to the tower base 1110. In other words, the saddle slide 1112 rotates by rotating the tower base 1110 with respect to the base ring 1108 and sweeps an arc by moving the saddle slide 1112 with respect to the tower base 1110. The saddle slide 1112 and the tower base 1110 are fixed in place by tightening of the thumbscrews 1114, which pulls the blocks 1118 against the base ring 1108, the base ring 1108 is pulled against the tower base 1110, and the tower base is pulled against the saddle slide.

The saddle assembly 1104 also includes a guide lumen 1120 having a saddle trajectory that passes through the base ring 1108 and the instrument immobilizer 1100. The guide lumen 1120 is dimensioned and configured to interchangeably retain alignment guides and instrument guides (described below). A thumbscrew 1122 or other fixation device extends through a wall of a cylindrical portion of the saddle slide 1112 that defines the guide lumen 1120. The thumbscrew 1122 is operable to engage and retain an alignment guide or instrument guide having a portion disposed within the guide lumen 1120. The saddle slide 1112 is positionable to orient the saddle trajectory in various orientations available with the above described arcuate and rotational movement. One example of the saddle assembly 1104 is further described in U.S. patent application Ser. No. 10/671,913, filed on Sep. 25, 2003, which is assigned to the assignee of the present application and which is incorporated by reference herein in its entirety. Additional examples of saddles are shown in U.S. patent application Ser. No. 09/828,451, filed on Apr. 6, 2001, which is assigned to the assignee of the present patent application, and which is incorporated by reference herein in its entirety.

FIG. 11A also illustrates an alignment ring 1136 including tabs 1138. The tabs 1138 are sized and shaped to engage with a rack 1140 including, for instance teeth 1142. The teeth 1142, in one example, are spaced around the rack 1140 at 4 degree intervals. The tabs 1138 deform with rotation of the alignment ring 1136 relative to the rack 1140 and snap into the grooves between the teeth 1142 to provide a clicking detent. The alignment ring 1136, in another example, is thus incrementally positionable around the rack 1140.

The alignment ring 1136 is sized and shaped to fit around the wall of the upwardly protruding cylindrical portion of the saddle slide 1112 that defines the guide lumen 1120. Clamps 1144 extend from the alignment ring 1136, in another example. The rack 1140 projects radially, in yet another example, from the cylindrical portion of the saddle slide 1112 and defines a lip. The clamps 1144 are sized and shaped to engage with the lip and secure the alignment ring 1136 to the saddle slide 1112 with inwardly extending hooks 1146, for example. The clamps 1144 deform as the hooks 1146 are pressed over the rack 1140. The clamps 1144 assume the undeformed shape when the alignment ring 1136 is pressed onto the rack 1140 and hooks 1146 disengage from the rack 1140 and engage against the lip to secure the alignment ring 1136 to the saddle slide 1112. An inner surface of the alignment ring 1136 defines grooves 1132 dimensioned and configured to receive keyed teeth from an alignment guide or instrument guide (both described below). In one example, the grooves 1132 are positioned every 45 degrees about the inner surface of the alignment ring 1136.

## 12

FIG. 11B illustrates another example of an alignment ring 1124 includes two semi-circular portions 1126. Each semi-circular portion 1126 is dimensioned and configured to fit around the wall of the upwardly protruding cylindrical portion of the saddle slide 1112 that defines the guide lumen 1120. This wall includes an inward turned lip dimensioned and configured to engage a groove present in each semi-circular portion 1126. In one example, the lip and grooves have cooperatively engaged teeth, spaced approximately every 6 degrees of the 360 degree cylindrical wall. The semi-circular portions 1126 are coupled to one another, such as with elastic bands 1128. The ends of the semi-circular portions 1126 have pinching surfaces 1130 that extend from the semi-circular portions 1126. Each pair of pinching surfaces 1130 is near one of the elastic bands 1128 on opposing sides of the elastic band 1128. Pressure applied to opposed pinching surfaces 1130 stretches the elastic band 1128 and separates the semi-circular portions 1126. In this way the pinching surfaces 1130 are operable to spread the semi-circular portions 1126 apart and allow rotational movement of the alignment ring 1124 with respect to the saddle slide 1112. An inner surface of the alignment ring 1124 defines grooves 1132 dimensioned and configured to receive keyed teeth from an alignment guide or instrument guide (both described below). In one example, the grooves 1132 are positioned every 45 degrees about the inner surface of the alignment ring 1124.

FIG. 12 shows an exploded view of the fixture assembly 102 including the saddle assembly 1104, alignment ring 1136, a centered alignment guide 1200, and an orienting fixture 1202. The centered alignment guide 1200 includes a base 1204 and an alignment pin 1206 coupled to the base. In this example, the alignment pin 1206 is centrally aligned with the base 1204 such that when the centered alignment guide 1200 is inserted into the lumen 1120 of the saddle assembly 1104, the pin 1206 is centered within the lumen 1120 to define the saddle trajectory. The centered alignment guide 1200 is immobilized within the lumen 1120 by thumbscrew 1122 or the like. In one example, the centered alignment guide 1200 includes keyed teeth 1208. The keyed teeth 1208 are dimensioned and configured to cooperatively engage the surfaces defining the grooves 1132 of the alignment ring 1136. This prevents undesired rotation between the saddle assembly 1104 and the centered alignment guide 1200. In one example, the keyed teeth 1208 are disposed around the circumference of the centered alignment guide 1200 at approximately 45 degree intervals. In one example, the centered alignment guide 1200 includes a flange 1210 that partially or completely circles a circumferential portion of the alignment guide 1200. The flange 1210 engages the upper surface of the cylindrical wall of the saddle slide 1112 that defines the guide lumen 1120. As a result, only the base 1204 is within the guide lumen 1120 when the centered alignment guide 1200 is coupled to the saddle assembly 1104.

The orienting fixture 1202 is coupled to the alignment pin 1206. In one example, a thumbscrew 1212 or other fixation device extends through a portion of the centered alignment guide base 1204 toward the alignment pin 1206. The thumbscrew 1212 is operable to engage and retain the orienting fixture 1202 against the alignment pin 1206. In one example, the orienting fixture 1202 is remotely detectable such as by remote positioning systems using infrared (IR) light detection. Such detection uses a number of detectable objects on the orienting fixture 1202. Examples of such objects include reflective structures or light emitting diodes (LED's) included on the orienting fixture 1202. In another embodiment, the remote detection of the detectable objects uses a tissue imaging method. Suitable tissue imaging methods include, but are

not limited to: magnetic resonance imaging (MRI); computed tomography (CT); ultrasound imaging; etc. In one example, the orienting fixture **1202** is used to locate and display the saddle trajectory on an image-guided surgical (IGS) computer workstation. In another example, the orienting fixture **1202** is used to compute the distance to a target in the brain from the orienting fixture. One suitable orienting fixture **1202** is the StealthFighter™, manufactured by Medtronic Inc. of Minneapolis, Minn.

In another example, the flange **1210** of alignment guide **1200** includes an alignment window **1214**. The alignment window **1214**, in one example, is a notch, opening or the like in the flange **1210**. The alignment ring **1136** includes markings **1216**, for instance alpha-numerical markings. Through cooperative engagement of the keyed teeth **1208** with the grooves **1132** (described above) the alignment window **1214** of the alignment guide **1200** reveals at least one marking **1216**. The keyed teeth **1208**, grooves **1132**, alignment window **1214**, and the markings **1216** are used cooperatively to position the alignment guide **1200**, and thus the orienting fixture **1202**, in a desired orientation within the guide lumen **1120**. The markings **1216** are positioned around the alignment ring **1136** to correspond, in one example, to the 45 degree increments between the keyed teeth **1208**. In another example, an offset alignment guide **1300** (described below) includes an alignment window **1214** similar to that of centered alignment guide **1200**. The alignment window **1214** and markings **1216** allow for accurate orientation of instrument lumens within an instrument guide (described below).

FIG. **13** is an exploded view of the fixture assembly **102** including the saddle assembly **1104**, alignment ring **1136**, an offset alignment guide **1300**, and an orienting fixture **1202**. The offset alignment guide **1300** is similar to the centered alignment guide **1200** described above, except that its alignment pin **1306** is offset from its central axis. The alignment pin **1306** is parallel to the central axis of the cylindrical base **1204** but offset therefrom. When the offset alignment guide **1300** is coupled to the saddle assembly **1104**, the pin **1306** defines a saddle trajectory offset from the center of the guide lumen **1120**. Multiple combinations of saddle trajectories are available with adjustments of the alignment ring **1136** and/or the offset alignment guide **1300**. In one example, the offset alignment guide **1300** is repositioned within the alignment ring **1136** with teeth **1208** at 45 degree increments around the 360 degree circle defined by the alignment ring **1136**. In another example, the alignment ring **1136** is rotated according to cooperatively engaged teeth (described above) incrementally spaced every 4 degrees and disposed within the inner groove of the alignment ring **1136** and lip of the saddle slide **1112**. In yet another example, the offset alignment guide **1300** is adjusted according to the teeth **1208** spaced every 45 degrees as well as the cooperatively engaged teeth between the alignment ring **1136** and the saddle slide **1112** to achieve additional saddle trajectories.

In another example, the flange **1210** of alignment guide **1300** includes an alignment window **1214** as described above regarding alignment guide **1200**. The alignment ring **1136** includes markings, for instance alpha-numerical markings **1216**. The keyed teeth **1208**, grooves **1132**, alignment window **1214**, and the markings **1216** are used cooperatively to position the alignment guide **1300** in a desired orientation within the guide lumen **1120**.

FIG. **14** is a partial sectional and exploded view of the fixture assembly **102** including the saddle assembly **1104**, alignment ring **1136**, and a centered instrument guide **1400**. In this example, the centered instrument guide **1400** includes a first portion **1402** and a second portion **1404**. The second

portion **1404** is coupled to the saddle assembly **1104** and immobilized by thumbscrew **1122**. Like the alignment guides **1200** and **1300**, the centered instrument guide **1400** includes keyed teeth **1406** dimensioned and configured to cooperatively engage the surfaces defining the grooves **1132** of the alignment ring **1136**. Relative rotation between the centered instrument guide **1400** and the saddle assembly **1104** is prohibited by the relationship of the keyed teeth **1406** to the surfaces defining the grooves **1132** and by the tabs **1138** on the alignment ring **1136** that engage corresponding teeth **1142** around the guide lumen **1120**. In one example, a flange **1408** is disposed substantially between the first portion **1402** and second portion **1404**. In another example, the flange **1408** is included in the first portion **1402** or second portion **1404**. The flange **1408** extends from and surrounds all or a portion of the centered instrument guide **1400**. The flange **1408** engages the upper surface of the alignment ring **1136** so only the second portion **1404** is within the guide lumen when the centered instrument guide **1400** is coupled to the saddle assembly **1104**.

In this example, a multilumen insert **1412** is disposed within a passage **1414** defined by an inner surface of the centered instrument guide **1400**. The multilumen insert **1412** is dimensioned and configured to snugly couple with the inner surface. Instrument lumens **1416** are arranged in a pattern within the insert **1412**. In this example, a central lumen **1416** extends substantially through the insert **1412** along a central axis of the insert **1412**. Four additional instrument lumens **1416** are disposed around the central lumen **1416** at 90 degree intervals. In another example, the instrument lumens **1416** are disposed in a different configuration within the insert **1412**, for example, in a pentagonal pattern or a three by three matrix of lumens **1416**. Each instrument lumen **1416** is dimensioned and configured to slidably couple with a guide tube (described below) while constraining lateral movement of the guide tube. In one example, the instrument lumens **1416** are defined by a single inner surface of the multi lumen insert **1412**. In other words, the lumens **1416** are furrows interconnected within the insert **1412**. In another example, the instrument lumens **1416** are separate and distinct lumens extending through the insert **1412**.

The first portion **1402** of centered instrument guide **1400** includes proximally accessible keyed teeth **1418**. The keyed teeth **1418** are disposed around the centered instrument guide **1400**. In one example, the keyed teeth **1418** are disposed at 90 degree intervals around the guide **1400**. In this example, the keyed teeth **1418** and the first portion **1402** are dimensioned and configured to couple with the normalizing stage apparatus **100**. The keyed teeth **1418** engage with corresponding slots **500** (See FIG. **5**) on the normalizing stage base **200** to prohibit undesirable relative rotation between the normalizing stage apparatus **100** and the centered instrument guide **1400**. The offset instrument guide (described below) also includes keyed teeth dimensioned and configured to couple with the normalizing stage base **200** and prohibit undesirable rotation between the normalizing stage apparatus **100** and the offset instrument guide.

In one example, the instrument guide **1400** includes at least one alignment window **1420** within the flange **1408**. The alignment window **1420** is sized and shaped to reveal markings **1216** on the alignment ring **1136** when the instrument guide **1400** is coupled to the alignment ring **1136**. In one example, the instrument guide **1400** is positioned on the alignment ring **1136** so the alignment window **1420** reveals the same marking **1216** determined with the alignment guide **1200**. The keyed teeth **1406** are disposed within the grooves **1132** of the alignment ring **1136** to orient the instrument guide

15

1400 on the alignment ring 1136. The instrument lumens 1416 are oriented in the instrument guide 1400 so matching of the marking 1216 exposed in the alignment window 1214 (alignment guide) to the marking 1216 exposed in the alignment window 1420 (instrument guide) positions the instrument lumens 1416 in the desired orientation. The orienting fixture 1202 is used to obtain the desired orientation of the instrument guide 1400 including the instrument lumens 1416. As a result, if the markings 1216 exposed in the alignment window 1420 are the same as those in alignment window 1214 the instrument lumens 1416 are in the desired orientation.

In another example, the instrument guide 1400 includes a skirt 1422. The skirt 1422 extends downwardly with respect to the flange 1408 and is sized and shaped to snugly couple around the alignment ring 1136. Coupling of the skirt 1422 around the alignment ring 1136 substantially prevents rotation of the alignment ring 1136 because the skirt 1422 pins the tabs 1138 against the rack 1140. As a result, the tabs 1138 are unable to deform and move around the teeth 1142. The skirt 1422 secures the instrument guide 1400 in a desired orientation determined, for example with the markings 1216 and the alignment window 1420 (described above).

FIG. 15 is a partial sectional and exploded view of the fixture assembly 102 including the saddle assembly 1104, alignment ring 1136, and an offset instrument guide 1500. The offset instrument guide 1500 is similar to the centered instrument guide 1400. In this example, the offset instrument guide 1500 includes a first portion 1502 and a second portion 1504. In a similar manner to the offset alignment guide 1300, the offset instrument guide 1500 is positionable to define multiple trajectories. The offset instrument guide 1500 is adjusted with positioning of the guide 1500 within the alignment ring 1136 to engage teeth 1406 with grooves 1132 and positioning of the alignment ring 1136 using tabs 1138 and corresponding teeth 1142 on the rack 1140 of the saddle slide 1112.

FIG. 16A shows an exploded view of the normalizing stage apparatus 100, a guide tube stop 1600, a guide tube 1602, and an obturator 1604. The guide tube stop 1600 is dimensioned and configured so its cylindrical outer surface fits snugly in the cylindrical inner surface that defines the guide tube stop lumen 216. In this example, a guide tube stop flange 1606 on the guide tube stop 1600 engages an upper lip of a surface that defines the lumen 216 of the first stage 210. In one example, guide tube lumens 1608 are arranged in a pattern within the guide tube stop 1600. In this example, a central lumen 1608 extends through the guide tube stop 1600 along a central axis of the guide tube stop 1600. Four additional guide tube lumens 1608 are disposed around the central lumen 1608 at 90 degree intervals. In another example, the guide tube lumens 1608 are disposed in a different configuration through the guide tube stop 1600, for example, in a pentagonal pattern or a three by three matrix of lumens 1608. In yet another example, the guide tube stop 1600 includes an outer ring having the flange 1606 and an insert dimensioned and configured to fit therein. The insert includes a pattern of guide tube lumens 1608. Different patterns of lumens 1608 are available in different inserts, which may be packaged together (and with any other components such as the normalizing stage) and sold as a kit. The instrument lumens 1608 are dimensioned and configured to slidably couple with the guide tube 1602 while constraining lateral movement of the guide tube 1602. In one example, the guide tube stop lumen 216 is keyed to the guide tube stop 1600. Such keying permits alignment of the pattern of lumens 1608 with the pattern of instrument lumens 1416 of the multi lumen insert 1412.

16

The guide tube 1602 snugly slides into one of the lumens 1608 of the guide tube stop 1600. In this example, a guide tube flange 1610 is substantially adjacent a proximal end of the guide tube 1602, and extends partially or completely around the guide tube 1602. The flange 1610 engages the upper surface of the guide tube stop 1600 when the guide tube 1602 is plunged through the guide tube stop 1600. This prevents the guide tube 1602 from sliding through the guide tube stop 1600. In this example, the guide tube 1602 is of a predetermined length, such that a physician or technician could use an "off the shelf" guide tube for a procedure with the normalizing stage with any patient. The guide tube distal end 1612 is plunged until the flange 1610 engages the guide tube stop 1600, in one example. When the first stage 210 is positioned at the proper distance to target and the flange 1610 has engaged the guide tube stop 1600, the distal end 1612 is substantially adjacent to the desired target. In one example, the distal end 1612 is then offset by a desired known distance from the target, for example 15 millimeters. In another example, the distal end 1612 is offset from the target a smaller increment according to the desires of the physician.

When initially plunging the guide tube 1602 the obturator 1604 is included within the guide tube. The obturator 1604 has an outer surface dimensioned and configured to slidably couple with the inner surface of the guide tube 1602. In this example, the obturator 1604 has a length substantially similar to the guide tube 1602. The distal ends of the obturator 1604 and guide tube 1602 define a blunt distal surface that prevents coring of the brain or other tissue. Near a proximal end of the obturator 1604 is an obturator flange 1616 that extends partially or completely around its circumference. The flange 1616 engages the upper surface of the guide tube 1602 when the obturator 1604 is within the guide tube. This prevents the obturator 1604 from sliding through the guide tube 1602.

FIG. 16B is an exploded view of one example of a guide tube stop 1620. The guide tube stop 1620 includes an outer ring 1622 sized and shaped so its cylindrical outer surface fits snugly in the cylindrical inner surface that defines the guide tube stop lumen 216 (FIGS. 2 and 16A). As described above for guide tube stop 1600, the outer ring 1622 of the guide tube stop 1620 includes a flange 1606 radially extending from the outer ring 1622. The flange 1606 engages an upper lip of a surface that defines the lumen 216 of the first stage 210. An inner surface 1624 of the outer ring 1622 defines at least two grooves 1626 sized and shaped to slidably couple with the guide tube 1602 (FIG. 16B).

The guide tube stop 1620 includes a rocker 1628 sized and shaped to fit within the outer ring 1622. The rocker 1628 includes at least two grooves 1630 sized and shaped to slidably couple with the guide tube 1602. The rocker 1628 further includes, in one example a projection 1632 extending toward the grooves 1626 of the outer ring 1622. The projection 1632 is operable to engage against the inner surface 1624 of the outer ring 1622 in one example. In another example, the projection 1632 engages against the guide tube 1602 disposed between the rocker 1628 and the inner surface 1624 to substantially immobilize the guide tube 1602. The rocker 1628 includes, optionally, a stud 1634. The stud 1634, in one example, is sized and shaped to extend at least partially through a notch 1636 in the outer ring 1622. The stud 1634 is engaged by a thumbscrew 1638 (FIG. 16A, 16B) that extends through a portion of the first stage 210 and into the lumen 216. The thumbscrew 1638 is operable to move the rocker 1628 by engaging the stud 1634. The rocker, in one example, moves toward the grooves 1626 of the outer ring 1622 and/or rotates around the stud 1634 so the projection 1632 engages against the outer ring inner surface 1624 or the guide tube 1602.



In another example, the guide tube stop 1620 includes a seat 1640 sized and shaped to fit between the inner surface 1624 including the grooves 1626 and the surface of the rocker 1628 that defines the grooves 1630. In one example, the seat 1640 includes legs 1642 sized and shaped to extend through the outer ring 1622. The legs 1642 include detents 1644 substantially adjacent to the free ends of the legs 1642. In another example, detents 1644 engage against the inner surface 1624 of the outer ring 1622 during insertion of the legs 1642 into the outer ring 1622. The legs 1642 correspondingly deform and snap into their original orientations once the detents 1644 exit the outer ring 1622. The detents 1644 securely couple the seat 1640 to the outer ring 1622. In another example, the detents 1644 cooperate with an upper surface 1646 of the seat 1640 to securely couple and retain the rocker 1628 and the seat 1640 within the outer ring 1622. In yet another example, the detents 1644 securely couple the seat 1640 to the outer ring and allow translational movement of the seat 1640 within the outer ring 1622.

The legs 1642 of the seat 1640 cooperate with the grooves 1630 of the rocker 1628 and the grooves 1626 of the outer ring 1622 to form the guide tube lumens 1608 (FIG. 16A). In one example, the projection 1632 of the rocker 1628 cooperates with the inner surface 1624 of the outer ring 1622 to define the central guide tube lumen 1608. In another example, the guide tube lumens 1608 are aligned with the pattern 1648 extending through the upper surface 1646.

When assembled, the guide tube stop 1620 operates to pass at least one guide tube 1602 through one of the guide tube lumens 1608. In one example, the guide tube lumens 1608 are sized and shaped so the guide tube 1602 is slidably coupled with the guide tube stop 1620. In another example, the guide tube lumens 1608 of the guide tube stop 1620 are aligned with the instrument lumens 1416 in the instrument guides 1400, 1500 (FIGS. 14 and 15) using corresponding keys and recesses included on the first stage 210 and the guide tube stop 1620. In yet another example, the thumbscrew 1638 is turned to clamp the guide tube stop around the guide tube 1602 and substantially immobilize the guide tube 1602 (described below). Immobilizing the guide tube 1602 substantially prevents undesirable movement of the guide tube 1602 such as during exchange of instruments when the instruments are drawn through the guide tube 1602.

In one example, the cooperative relationship of the rocker 1628 with the outer ring 1622 and the seat 1640 facilitates clamping of the guide tube 1602 in any of the guide tube lumens 1608. In one example, a guide tube 1602 is inserted through the pattern 1648 into the guide tube lumens 1608. The thumb screw 1638 is operated to engage the stud 1634 and move the rocker 1628 toward the grooves 1626 of the outer ring 1622. Where the guide tube 1602 is disposed within one of the guide tube lumens 1608 between the rocker 1628 and the seat 1640, the rocker 1628 moves until the opposing surfaces defining the grooves 1630 and the legs 1642 engage against and securely clamp around the guide tube 1602. In another example, the guide tube 1602 is disposed between the projection 1632 and the inner surface 1624 substantially adjacent to the grooves 1626. The rocker 1628 moves toward the inner surface 1624 and clamps the guide tube 1602 between the projection 1632 and the inner surface 1624. In one example, the rocker 1628 pivots around the stud 1634 to engage and clamp the guide tube 1602. In yet another example, the guide tube 1602 is disposed between the legs 1642 and the grooves 1626. The rocker 1628 moves and engages against the seat 1640. The seat 1640 moves with the rocker 1628 toward the grooves 1626. The guide tube 1602 is clamped between the legs 1642 and the inner surface 1624

defining the grooves 1626. The guide tube stop 1620 is thereby operable to clamp and immobilize the guide tube 1602, including multiple guide tubes 1602, in any of the guide tube lumens 1608.

FIG. 17 is a perspective view of the normalizing stage 100 arranged for advancing a first instrument 1700, for example a recording electrode. In this example, the guide tube stop 1600 is coupled to the first stage 210, as described above. The guide tube 1602 extends through the guide tube stop 1600 and the first stage 210. The guide tube flange 1610 prevents the guide tube 1602 from sliding completely through the guide tube stop 1600. A spacer tube 1702 is positioned within the guide tube 1602 and is dimensioned and configured to slidably couple with the inner surface of the guide tube 1602. The spacer tube 1702 includes a spacer tube flange 1704 extending partially or completely about its proximal circumference. The flange 1704 engages the upper surface of the guide tube 1602 when the spacer tube 1702 is within the guide tube 1602 and prevents the spacer tube from sliding through the guide tube 1602.

The first instrument 1700 is fed through the spacer tube 1702 toward the target. The spacer tube 1702 constrains lateral movement of the first instrument 1700. Therefore, the first instrument moves along the trajectory 228 defined by the socket 202 (or parallel to the trajectory 228 when using an offset lumen 1608) because the guide tube 1602 and spacer tube 1702 are aligned with that trajectory 228. A portion of the first instrument 1700 is immobilized within a retaining assembly 1706 that is coupled to the second stage 218 within the retaining assembly orifice 226. The thumbscrew 232 tightens the retaining assembly around the first instrument 1700. The retaining assembly 1706 immobilizes the portion of the first instrument 1700 with respect to the second stage 218. As a result, translation of the second stage 218 correspondingly translates the first instrument 1700 within the spacer tube 1702 and guide tube 1602.

FIG. 18 is a front view of a bracket assembly 1800 including a bracket 1802, a measurement tube 1804, and a second instrument 1806, for example a stimulation electrode. In this example, the bracket has a distal collar base 1808 dimensioned and configured to snugly couple with the second stage 218 within the retaining assembly orifice 226. A measurement tube lumen extends through the collar base 1808 at the distal end of the bracket 1802. The measurement tube lumen is dimensioned and configured to couple with a measurement tube 1812. The measurement tube 1812 extends from a proximal end 1814 to a distal end 1816. The proximal end 1814 is coupled to the bracket 1802 at the bracket proximal end against retaining prongs 1818. In this example, four prongs 1818 extend from each side of the bracket 1802. The inner surfaces of the prongs couple with the proximal end 1814 of the measurement tube 1812. In another example, additional or fewer prongs 1818 are included with the bracket 1802. In yet another example, each side of the bracket 1802 is dimensioned and configured to couple with the measurement tube 1812. In this example, the proximal end of the bracket 1802 immobilizes a portion of the second instrument 1806 with a thumbscrew 1820 or the like that extends through one side of the bracket into a furrow 1822 carrying the second instrument. The thumbscrew 1820 is rotated until one end engages the second instrument 1806 and immobilizes the instrument 1806 against the opposing side of the bracket 1802.

The measurement tube 1812 is used to calibrate the operating length of the second instrument 1806. The second instrument 1806 is positioned within the measurement tube 1812 and immobilized by the thumbscrew 1820 so a distal end of the second instrument is substantially coterminous

with the distal end **1816** of the measurement tube. The calibration of the second instrument **1806** length with respect to the measurement tube **1812** allows the distal end of the second instrument to plunge to the target area determined with the first instrument (described below). Additionally, the bracket **1802** provides additional instrument length for the guide tube **1602** to advance along, as described below. The measurement tube **1812** eliminates the need for measuring out the second instrument **1806** thereby simplifying the determination of the second instrument **1806** length.

#### Operation of the Normalizing Stage Assembly with Centered Alignment Guides and Centered Instrument Guides

In one example of operation, a burr hole is cut into the skull of the patient. As shown in FIG. **11**, the instrument immobilizer **1100** is coupled to the skull around the burr hole. In an example, the instrument immobilizer **1100** is coupled to the skull with bone screws. Then, the saddle assembly **1104** is coupled to the instrument immobilizer **1100**, such as by screws extending through the base ring **1108**. The alignment ring **1136** is disposed around the cylindrical wall defining the guide lumen **1120**. The alignment ring **1136** engages the inward turned lip of the saddle slide **1112**, as described above. As shown in FIG. **12**, the centered alignment guide **1200** is disposed within the guide lumen **1120**. The centered alignment guide keyed teeth **1208** engage the corresponding grooves **1132** of the alignment ring **1136**. The engagement of the keyed teeth **1208** to the grooves **1132** and the engagement of the alignment ring **1136** to the rack **1140** of the saddle slide **1112** prevents unwanted rotation between the centered alignment guide **1200** and the saddle assembly **1104**.

The orienting fixture **1202**, illustrated in FIG. **12**, is coupled to the alignment pin **1206**. In this example, the alignment guide thumbscrew **1212** immobilizes the orienting fixture **1202** between the thumbscrew and the alignment pin **1206**. The saddle assembly **1104** is then adjusted rotationally, arcuately, or both to define a trajectory to a desired target of the brain. The orientation fixture **1202** is used to display the trajectory on an IGS workstation during the adjustment. Once the desired trajectory is obtained thumbscrews **1114** are tightened on the saddle assembly **1104** to prevent further rotational and arcuate motion of the saddle assembly **1104**. The alignment guide **1200** and alignment ring **1136** are rotated around guide lumen **1120**. In one example, the tabs **1138** and teeth **1142** of the rack **1140** cooperatively engage for rotation of the alignment guide **1200** and the alignment ring **1136** at clicking increments (e.g. 4 degree increments). A marking **1216** is revealed through the alignment window **1214**. The alignment guide **1200** and alignment ring **1136** are rotated so the marking **1216** and thereby the alignment guide **1200** coupled to the alignment ring **1136** are in a desired orientation (e.g., an anterior-to-posterior orientation of a skull). As a result, the pattern of instrument lumens **1416** (See FIG. **14**) will be in the same desired orientation when the instrument guide **1400** is coupled to the alignment ring **1136** (described below).

Alignment of the alignment guide **1200** and the alignment ring **1136** to the desired orientation is done visually in one example. In another example, an IGS workstation is used to measure rotation of the alignment guide **1200** and the alignment ring **1136** and to determine when the desired orientation is achieved. The orienting fixture **1202** is keyed to the alignment guide **1200** in this example, to align the orienting fixture **1202** with respect to the alignment guide **1200**.

The relative location of the orienting fixture **1202** is also used by the IGS workstation to determine the proper location of the first stage **210** with respect to the desired target area,

and proper lengths of instruments **1700**, **1806**, and the guide tube **1602**, obturator **1604** and spacer tube **1702**. In one example, the IGS workstation determines the initial position of the first stage **210** with respect to the target area. The first stage **210** is moved with respect to the base **200** and the position of the first stage **210** relative to the target area is determined with, for instance, the scale **304** and reference mark **306** (described below)

FIG. **19** is a perspective view illustrating the fixture assembly **102**, normalizing stage assembly **100**, and a first instrument **1700**. The orienting fixture **1202** and the centered alignment guide **1200** have been removed from the saddle assembly **1104**. The centered instrument guide **1400** is then coupled to the saddle assembly **1104** in a similar manner to the centered alignment guide **1200**. The centered instrument guide **1400** is coupled to the alignment ring **1136** so the same marking **1216** used to position the alignment guide **1200** and the alignment ring **1136** is revealed in the alignment window **1420**. The centered instrument guide **1400** is thereby positioned in the desired orientation determined with the alignment guide **1200** and the orientation fixture **1202** (described above). Revealing the same marking **1216** ensures proper positioning of the instrument guide **1400** and the corresponding instrument lumens **1416** to the desired orientation.

The first stage actuator **300** (FIG. **3**) is turned to initially adjust the first stage **210** to substantially coincide with the desired distance as determined with the orienting fixture **1202**. The scale **304** and reference mark **306** are used to measure the position of the first stage **210** with respect to the desired target area. If necessary, the second stage **218** is adjusted with the actuator knob **308** to a desired starting position. In one example, the starting position for the second stage **218** is read from the scales **316A-C**, attached to the first stage **210**, and a reference marking **314**, attached to a protrusion **310** extending from the second stage **218**. In another example, the position of the second stage **218** is determined with the potentiometer assembly **600**.

In one example, the stages **210**, **218** are adjusted before coupling the normalizing stage apparatus **100** to the centered instrument guide **1400**. In another example, the adjustments are made after coupling the normalizing stage **100** to the centered instrument guide **1400**. Keyed teeth **1418** on the centered instrument guide **1400** engage with corresponding slots **500** within the socket **202** of the base **200**. The keyed teeth **1418** and slots **500** prevent relative rotation between the centered instrument guide **1400** and the normalizing stage assembly **100**. Thumbscrew **204** is tightened to securely couple the normalizing stage **100** to the centered instrument guide **1400**.

In FIG. **16A**, the guide tube **1602** and obturator **1604** are coupled to each other, so the obturator is disposed within the guide tube **1602** and the obturator flange **1616** engages the upper surface of the guide tube. The guide tube distal end **1612** and obturator distal end **1614** define a blunt surface. Both the guide tube **1602** and obturator **1604** are of a standard length that is factored into the function used to determine the position of the first stage **210** with the orienting fixture **1202** (FIG. **12**). The guide tube **1602** and obturator **1604** are plunged through a guide tube lumen **1608** within the guide tube stop **1600**. The guide tube flange **1610** engages the guide tube stop **1600** to prevent unwanted advancement of the guide tube **1602** beyond the guide tube stop **1600**. The guide tube **1602** and obturator **1604** also extend through the centered instrument guide **1400**, specifically, one of the instrument guide lumens **1416**. In this example, because the first stage **210** is adjusted to substantially coincide with the distance measurement described above, the distal ends of the standard

length guide tube **1602** and obturator **1604**, are substantially adjacent to the desired target when plunged. In one example, these distal ends are offset a desired approach distance from the target, for example, 15 millimeters. In another example, the physician offsets the distal ends a desired approach distance.

After plunging of the guide tube **1602** and obturator **1604**, the obturator **1604** is removed from the guide tube **1602**, such as by grasping the obturator flange **1616** by hand or with a tool such as a forceps to lift the obturator **1604** out of the guide tube **1602**.

After removal of the obturator **1604**, the spacer tube **1702** (FIG. 17) is then inserted into the guide tube **1602** until the spacer tube flange **1704** engages the upper surface of the guide tube **1602**. The spacer tube **1702** has a length substantially similar to that of the guide tube **1602**. As a result, the distal end of the spacer tube **1702** is substantially adjacent to the distal end of the guide tube **1602**.

As shown in FIG. 17, the retaining assembly **1706** is then inserted into the retaining assembly lumen **226** of the second stage **218**. The first instrument **1700** is fed through the retaining assembly **1706** and into spacer tube **1702**. In this example, the thumbscrew **232** is rotated to tighten the retaining assembly **1706** around the first instrument **1700**. The first instrument **1700** is of a standard predetermined length, for such an off the shelf instrument **1700**. In one example, the first instrument **1700** is a recording electrode with a flange **1708** at its proximal end to engage an upper surface of the retaining assembly **1706**. The distance between a distal end of the instrument and the flange is a standard predetermined length. The first stage **210** and second stage **218** are initially positioned to take into account the distance to the desired target and the predetermined lengths of the instruments and tubes (described above). As a result, the distal end of the standard length first instrument **1700**, when plunged with the flange **1708** engaged to the retaining assembly **1706**, is substantially adjacent to the distal end of the guide tube **1602** and the distal end of the spacer tube **1702**. The distal end of the first instrument **1700** and the distal end of the guide tube **1602** are substantially adjacent to the desired target or are offset from the desired target area some distance, for example, 15 millimeters, as described above.

In this example, a physician or technician then operates actuator knob **308** to move the second stage **218** and first instrument **1700** coupled thereto along the screw **220**. The distal end of the first instrument **1700** is moved toward, away or through the desired target, as desired. In one example, the relative position of the distal end of the first instrument **1700** with respect to the desired target area is read from the scale **316A** with reference marking **314**. In another example, the relative position of the first instrument **1700** is read from the reference marking **402** against the fine scale **400** (FIG. 4) coupled to the screw **220**. In still another example, the relative position of the first instrument **1700** is measured with a potentiometer assembly **600**, as described above. In another embodiment the hydraulic system **700** is used to move the second stage **218** through actuation of the master piston **708** with respect to the master cylinder **706**.

If the physician is satisfied with the track of the first instrument **1700** to the desired target, a second instrument **1806** is substituted (described below). If the physician is not satisfied with the track of the first instrument **1700** (for example, a blood vessel blocks advancement of the first instrument **1700**) it is retracted away from the target. The retaining assembly **1706** is loosened through thumbscrew **232**, and the first instrument **1700** is removed from the normalizing stage assembly **100**. The retaining assembly **1706** is then removed

from the second stage **218**. The guide tube **1602** and spacer tube **1702** are then removed from the guide tube stop **1600**. The physician may then plunge another guide tube **1602** and obturator **1604** in an adjacent guide tube lumen **1608**. The process described above is then substantially repeated for the new track created by the guide tube **1602** in the adjacent lumen **1608**.

#### Operation of the Normalizing Stage Assembly with Offset Alignment Guides and Offset Instrument Guides

Alternatively, the physician removes the entire normalizing stage assembly **100**, and the centered instrument guide **1400**. An offset alignment guide **1300** (FIG. 13) is coupled to the saddle assembly **1104**. In another example, the physician uses the offset alignment guide **1300** from the beginning instead of the centered alignment guide **1200**, if so desired. The keyed teeth **1214** of the offset alignment guide **1300** and the corresponding grooves **1132** on the alignment ring **1136** make the offset guide **1300** positionable at 45 degree increments (FIG. 11). Additionally, the offset alignment guide **1300** is positionable at 4 degree increments through actuation of alignment ring **1136** around the rack **1140**. The orienting fixture **1202**, illustrated in FIG. 12, is coupled to the alignment pin **1306**. In this example, the alignment guide thumbscrew **1212** immobilizes the orienting fixture **1202** between the thumbscrew and the alignment pin **1306**.

The saddle assembly **1104** is then adjusted rotationally and/or arcuately, to define a trajectory to a desired target of the brain. Once the physician is initially satisfied with the trajectory of the saddle assembly **1104** and offset alignment guide **1300** coupled thereto, thumbscrews **1114** are tightened on the saddle assembly **1104** to prevent further rotational and arcuate motion of the saddle **1104**. The location of the orienting fixture **1202** with respect to the desired target is detected through the imaging methods described above. The relative location of the orienting fixture **1202** is used to determine the desired location of the first stage **210** with respect to the target. An IGS work station, for example, takes into account the lengths of standardized "off the shelf" instruments **1700**, **1806**, and the guide tube **1602**, obturator **1604** and spacer tube **1702**.

The alignment guide **1300** and alignment ring **1136** are rotated around guide lumen **1120** as described above with the alignment guide **1200**. A marking **1216** is revealed through the alignment window **1214**. The alignment guide **1300** and alignment ring **1136** are rotated so the marking **1216** and thereby the alignment guide **1300** coupled to the alignment ring **1136** are in a desired orientation (e.g., an anterior-to-posterior orientation of a skull). As a result, the pattern of instrument lumens **1416** (See FIG. 15) will be in the same desired orientation when the instrument guide **1500** is coupled to the alignment ring **1136** (described below). Aligning of the alignment guide **1300** and the alignment ring **1136** to the desired orientation is done, for instance, visually or with an IGS workstation as described above for alignment guide **1200**.

The orienting fixture **1202** and the offset alignment guide **1300** are removed from the saddle assembly **1104**. The offset instrument guide **1500** is coupled to the saddle assembly **1104** in the same orientation as was the offset alignment guide **1300**. In one example, the offset instrument guide **1500** is coupled to the alignment ring **1136** so the same marking **1216** used to position the alignment guide **1300** and the alignment ring **1136** is revealed in the alignment window **1420**. The offset instrument guide **1500** is thereby positioned in the desired orientation determined with the alignment guide **1300** and the orientation fixture **1202** (described above). Revealing

the same marking **1216** ensures proper positioning of the instrument guide **1500** and the corresponding instrument lumens **1416** to the desired orientation.

The first stage actuator **300** is turned to initially adjust the first stage **210** to substantially coincide with the distance determined with the orienting fixture **1202**. The scale **304** and reference mark **306** are used to measure the position of the first stage **210** with respect to the desired target. If necessary, the second stage **218** is adjusted with the actuator knob **308** to a desired starting position. In one example, the starting position for the second stage **218** is read from one of the scales **316A-C**, attached to the first stage **210**, and a reference marking **314**, attached to a protrusion **310** extending from the second stage **218**. In another example, the position of the second stage **218** is determined with the potentiometer assembly **600** (FIG. 6) coupled between the second stage **218** and the first stage **210**.

The normalizing stage apparatus **100** is coupled to the offset instrument guide **1500** (See FIG. 15). In this example, the adjustments to the stages **210**, **218** are performed before coupling the normalizing stage apparatus **100** to the offset instrument guide **1500**. In another example, the adjustments are made after coupling the normalizing stage **100** to the offset guide **1500**. Keyed teeth **1510** on the offset guide **1500** engage with corresponding slots **500** within the socket **202** of the base **200**. This prevents relative rotation between the offset instrument guide **1500** and the normalizing stage assembly **100**. Thumbscrew **204** is tightened to securely couple the normalizing stage **100** to the offset instrument guide **1500**.

The obturator **1604** is inserted into the guide tube **1602** until the obturator flange **1616** engages the upper surface of the guide tube **1602**. The guide tube distal end and obturator distal end define a blunt surface. Both the guide tube **1602** and obturator **1604** are of a standard length that is factored into the function used to determine the position of the first stage **210** with the orienting fixture **1202**. The guide tube **1602** and obturator **1604** are plunged together through a guide tube lumen **1608** within the guide tube stop **1600** until the guide tube flange **1610** engages the guide tube stop **1600**. The guide tube **1602** and obturator **1604** also extend through the offset instrument guide **1500**, specifically, one of the instrument guide lumens **1416**. In this example, because the first stage **210** is adjusted to substantially coincide with the distance measurement described above, the distal ends of the standard length guide tube **1602** and obturator **1604**, are substantially adjacent to the desired target area when plunged. In one example, the distal ends are offset from the target a desired approach distance, for example, 15 millimeters. In another example, the physician offsets the distal ends a desired approach distance from the target.

After plunging of the guide tube **1602** and obturator **1604**, the obturator **1604** is removed from the guide tube **1602**. The spacer tube **1702** is inserted into the plunged guide tube **1602** until the spacer tube flange **1704** engages the upper surface of the guide tube **1602**. The spacer tube **1702** has a length substantially similar to that of the guide tube **1602** so the distal end of the spacer tube **1702**, when inserted, is substantially adjacent to the distal end **1612** of the guide tube **1602**.

FIG. 19 is a perspective view of the normalizing stage apparatus **100** showing the relation of the first instrument **1700** to the normalizing stage apparatus **100**. Operation of the normalizing stage apparatus **100** with the illustrated centered instrument guide **1400** is substantially similar to operation with the offset instrument guide **1500**. The retaining assembly **1706** is coupled to the second stage **218** and within retaining assembly orifice **226** after removal of the obturator **1604**.

The first instrument **1700** is then fed through the retaining assembly **1706** in the second stage **218** and into spacer tube **1702**. In this example, the thumbscrew **232** is rotated to tighten the retaining assembly **1706** around the first instrument **1700**. The first instrument **1700** is of a standard length. In one example, the first instrument **1700** is a recording electrode. In this example, the recording electrode has a distal end, and a flange **1708** disposed at its proximal end to engage an upper surface of the retaining assembly **1706**. The distance between the distal end of the instrument **1700** and the flange **1708** is a standard length. The first stage **210** and second stage **218** are initially positioned with respect to the desired target. The positioning of the first stage **210** and second stage **218** takes into account the lengths of the standardized (off the shelf) instruments and tubes (described above). As a result, the distal end of the standard length first instrument **1700**, when plunged with the flange **1708** engaged to the retaining assembly **1706**, is substantially adjacent to the distal end **1612** of the guide tube **1602** and the distal end of the spacer tube **1702**. In one example, the distal end of the first instrument **1700** and the distal end of the guide tube **1602** are substantially adjacent to the desired target. In another example, the distal end **1612** and distal end of the first instrument **1700** are offset from the desired target some distance, for example, 15 millimeters, as described above.

In this example, a physician or technician then turns actuator knob **308** to move the second stage **218**, and first instrument **1700** coupled thereto, along the screw **220**. The distal end of the first instrument **1700** is moved toward, away or through the desired target area as desired. In one example, the relative position of the distal end of the first instrument **1700** with respect to the desired target is read from the scale **316A** with reference marking **314**. In another example, the relative position of the first instrument **1700** distal end is read on the scale **316** with respect to the distal end of the guide tube **1602**. In yet another example, the relative position of the first instrument **1700** is read from the reference marking **402** against the fine scale **400** (FIG. 4) coupled to the screw **220**. In still another example, the relative position of the first instrument **1700** is measured with a potentiometer assembly **600**, as described above. In another embodiment the hydraulic system **700** is used to move the second stage **218** through actuation of the master piston **708** with respect to the master cylinder **706**.

If the physician is satisfied with the track of the first instrument **1700** to the desired target, a second instrument **1806** is substituted (described below). If the physician is not satisfied with the track of the first instrument **1700** (for example, a blood vessel blocks advancement of the first instrument **1700**) it is retracted away from the target. The retaining assembly **1706** is loosened through thumbscrew **232**, and the first instrument is removed from the normalizing stage assembly **100**. The retaining assembly **1706** is then removed from the second stage **218**. The guide tube **1602** and spacer tube **1702** are then removed from the guide tube stop **1600**. The physician may then plunge another guide tube **1602** and obturator **1604** in an adjacent guide tube lumen **1608**. The process described above is then substantially repeated for the new track created by the guide tube **1602** in the adjacent lumen **1608**. In another example, the physician adjusts the position of the offset instrument guide **1500** through actuation of the alignment ring **1136**. In one example, adjustment of the guide **1500** position also requires use of the offset alignment guide **1300** to redetermine the relative position of the first stage **210** with respect to the target area and standardized instruments and tubes. In still another example, the physician removes the offset instrument guide **1500** and uses a centered alignment

guide **1200** and centered instrument guide **1400** to make another track to the desired target area.

#### Operation of the Normalizing Stage Assembly with the Second Instrument

FIG. **20** is a perspective view showing the normalizing stage apparatus **100**, bracket assembly **1800**, and the second instrument **1806**. Before coupling of the bracket **1802** to the normalizing stage apparatus, the bracket assembly **1800** is used to measure out the length for the second instrument **1806**. The measurement tube **1804** (FIG. **18**) is coupled to the bracket **1802** so the tube is disposed within the measurement tube lumen **1810** and the proximal end **1814** of the tube is coupled to the bracket by the retaining prongs **1818**. The second instrument **1806** is fed into the measurement tube **1804** until the distal end of the second instrument is substantially coterminous with the distal end **1816** of the measurement tube (FIG. **18**). A portion of the second instrument **1806** is immobilized by thumbscrew **1820** that engages the second instrument **1806** against the opposing side of the bracket **1802**. The measurement tube is then uncoupled from the bracket **1802**. The retaining assembly **1706** is uncoupled from the second stage **218**, and the spacer tube **1702** is removed from engagement with the guide tube **1602** in a similar manner as the obturator **1604**. The bracket **1802** is coupled to the second stage within the retaining assembly orifice **226**. In this example, the retaining assembly orifice **226** includes a slot and the bracket collar base **1808** includes a key dimensioned and configured to cooperatively engage the surface defining the slot. The thumbscrew **232** is tightened to securely couple the bracket **1802** to the second stage. The slot and key relationship determines the orientation of the bracket **1802** relative to the second stage **218**. The second instrument **1806** is then fed, distal end first, through the guide tube **1602** and plunged toward the target along the track determined with the first instrument **1700**.

The bracket **1802** provides a constant offset distance between the second stage **218** and the bracket proximal end where the second instrument **1806** is coupled. This constant offset distance is reflected in the additional length of the second instrument **1806** over the first instrument **1700**. The constant offset allows the distal end of the second instrument **1806** to plunge to the location determined with the first instrument **1700**. In other words, when plunging the second instrument **1806**, the normalizing stage apparatus **100**, specifically first stage **210** and second stage **218**, are in the positions determined with the first instrument **1700**. The second instrument **1806** thus plunges so the distal end of the instrument is substantially adjacent to the prior location of the first instrument **1700** distal end.

A perspective view of the normalizing stage apparatus **100**, the second instrument **1806**, the guide tube **1602**, and the instrument immobilizer **1100** is shown in FIGS. **21** and **22**. The second instrument **1806** is disposed within the guide tube **1602**. To remove the guide tube **1602** and leave the second instrument **1806** at the desired location, the guide tube **1602** is moved out of engagement with the guide tube stop **1600**. The guide tube **1602** is advanced along the second instrument **1806** which is slidably coupled thereto. As shown in FIG. **21**, the guide tube **1602** is moved at least until the distal end of the guide tube is above the instrument immobilizer **1100**. The retaining piece **1106** is then moved into engagement against the second instrument **1806** to immobilize the instrument between the retaining piece and the opposing surface of the instrument immobilizer **1100**, as shown in FIG. **22**. The second instrument **1806** is substantially immobilized between the instrument immobilizer **1100** and the distal end of the

second instrument **1806**. Additionally, the distal end of the second instrument **1806** is located at the desired target location along the track determined with the first instrument **1700**.

The thumbscrew **1820** is loosened to release the second instrument **1806** from engagement to the bracket **1802**. In this example, the thumbscrew **204** is loosened to allow uncoupling of the normalizing stage assembly **100** from the instrument guide (**1600** or **1500**). The saddle assembly **1104** is uncoupled from the instrument immobilizer **1100** by loosening screws extending therebetween, in one example. In another example, the saddle assembly **1104** is uncoupled from the instrument immobilizer **1100** while the normalizing stage assembly **100** is still coupled to the saddle assembly **1104**. In yet another example, the second instrument **1806** is pulled through an orifice between the saddle slide **1112** and the tower base **1110** to uncouple the second instrument from the normalizing stage assembly **100**. The saddle assembly **1104** and normalizing stage assembly **100** are then easily uncoupled from the instrument immobilizer **1100** and the second instrument **1806** is not otherwise disturbed. The second instrument **1806** is left engaged to the instrument immobilizer with the distal end at the desired target.

FIG. **23** is a perspective view showing the instrument immobilizer **1100**, the second instrument **1806**, and a cap **2300**. The portion of the second instrument **1806** outside of the skull and beyond the instrument immobilizer **1100** is bent over, and the cap **2300** is engaged to the instrument immobilizer. In this example, the cap is elastic and deforms to snugly engage with the instrument immobilizer **1100** and retain the second instrument **1806** in its orientation.

#### Techniques for Using a Normalizing Stage Apparatus

FIG. **24** is a block diagram illustrating generally, by way of example, but not by way of limitation, examples of certain techniques for using a normalizing stage, such as the normalizing stage apparatus **100** of FIG. **1**. The normalizing stage, in this example, includes a base, a first stage moveably coupled to the base and operable to move with respect to the base, and a second stage moveably coupled to the first stage and operable to move with respect to the first stage and the base. The techniques disclosed herein need not be carried out in the exact order illustrated in the block diagrams of FIGS. **24-29**. At **2402**, a fixing assembly is coupled to the body. In this example, the fixing assembly is coupled to the skull. At **2404**, the relative position of the normalizing stage with respect to a desired target, the instruments, and other equipment (described above) is determined. A first instrument is plunged and advanced to the target at **2406**. In this example, the first instrument is a recording electrode. At **2408**, a second instrument is plunged to the target area. In this example, the second instrument is a stimulation electrode. At **2410**, the second instrument is immobilized and the normalizing stage and fixing assembly are removed.

FIG. **25** is a more detailed block diagram illustrating techniques for coupling the fixing assembly to the skull **2402**. At **2500**, an instrument immobilizer is coupled to the skull. In this example, the instrument immobilizer is coupled around a burr hole in the skull. A saddle is coupled to the instrument immobilizer at **2502**. In this example, the saddle is aligned with a trajectory defined by the instrument immobilizer. At **2504**, an alignment ring, such as the alignment ring **1136** in FIG. **11**, is coupled to the saddle.

FIG. **26** is a more detailed block diagram illustrating techniques for determining the relative position of the normalizing stage with respect to the desired target area, the instruments, and other equipment **2404**. At **2600**, an alignment guide is coupled to the saddle and engaged to the alignment

27

ring. In one example, the alignment guide is an embodiment such as centered alignment guide **1200**. The alignment guide includes an alignment pin aligned with the longitudinal axis of the alignment guide. In another example, the alignment guide includes an alignment pin parallel to, and offset from, the longitudinal axis of the alignment guide. At **2602**, an orienting fixture, such as orienting fixture **1202**, is coupled to the alignment guide. In one example, the orienting fixture is coupled to the alignment pin of the alignment guide. At **2604**, the saddle and the alignment ring are adjusted to determine a trajectory and orientation to the desired target. In this example, the saddle is adjusted rotationally and/or arcuately. The location of a first stage of the normalizing stage is determined with respect to the desired target, standardized (off the shelf) instruments, and tubes used to plunge the instruments, at **2606**. In this example, the location of the first stage is determined with imaging of the orienting fixture. At **2608**, the orienting fixture and alignment guide are uncoupled and removed.

FIG. **27** is a more detailed block diagram illustrating techniques for plunging the first instrument and advancing it toward the target area **2406**. At **2700**, the first stage is positioned to the desired starting position determined in **2404** (described above). At **2702**, the second stage is positioned to a desired starting position. In one example, the second stage is not adjusted because it is already calibrated to a starting position and is moveably coupled to the first stage. In this example, the second stage moves correspondingly with the first stage as the first stage is moved. At **2704**, an instrument guide is coupled to the saddle and engages with the alignment ring. In one example, the instrument guide has at least one instrument guide lumen aligned with the longitudinal axis of the instrument guide, as described with centered instrument guide **1400** above. In another example, the instrument guide includes at least one instrument guide lumen parallel to, and offset from, the longitudinal axis of the instrument guide. In yet another example, the offset instrument guide lumen has substantially the same alignment as the alignment pin of the offset alignment guide (described above). At **2706**, the normalizing stage is coupled to the instrument guide. In this example, the normalizing stage has a base that defines a trajectory, and the trajectory is parallel to the longitudinal axis of the instrument guide. In another example, the trajectory of the normalizing base is aligned with the longitudinal axis of the instrument guide. At **2708**, a standard length (usable off the shelf) guide tube and standard length (also usable off the shelf) obturator are plunged together through a guide tube stop coupled to the first stage of the normalizing stage until engaged to the guide tube stop. In this example, the obturator is coupled with the guide tube so the distal ends of the guide tube and obturator define a blunt surface. The obturator is removed from engagement with the guide tube at **2710**. At **2712**, a standard length off the shelf spacer tube is plunged through the guide tube stop, specifically the guide tube, until engaged with the guide tube. In this example, the guide tube, obturator, and spacer tube include flanges that engage surfaces, for example the guide tube stop, and prevent further plunging of the guide tube, obturator and/or spacer tube. At **2714**, the first instrument is plunged through a retaining assembly coupled to the second stage and the spacer tube toward the target. Because of the positioning of the first stage **2700** (and second stage **2702** if necessary), the first instrument distal end is coterminous with the distal end of the guide tube when plunged. At **2716**, the first instrument is moved toward, away and/or through the desired target. In this example, the first instrument is moved outside of the guide tube and toward the target area.

28

FIG. **28** is a more detailed block diagram illustrating techniques for plunging the second instrument **2408**. At **2800**, the first instrument is uncoupled and removed from the second stage retaining assembly and the spacer tube. At **2802**, the spacer tube is removed from engagement with the guide tube. In this example, the spacer tube is removed from the guide tube. At **2804**, a length of the second electrode is measured with a bracket (for example, bracket **1802**) and measurement tube (e.g. measurement tube **1804**) coupled to the bracket. In this example, the second instrument is fed through the measurement tube and the portion of the bracket coupled to the measurement tube. The second instrument is coupled to the bracket and the measurement tube is uncoupled from the bracket at **2806**. At **2808**, the bracket is coupled to the second stage of the normalizing stage. In this example, the retaining assembly is uncoupled from the second stage and the bracket coupled in its place. At **2810**, the second instrument is plunged through the guide tube toward the target along the track determined with the first instrument.

FIG. **29** is a more detailed block diagram illustrating techniques for immobilizing the second instrument and removing the stage and fixing assembly **2410**. At **2900**, the guide tube is moved out of engagement with the guide tube stop. In this example, the guide tube is advanced upward relative to the second stage along the second instrument. At **2902**, the instrument immobilizer (for example, instrument immobilizer **1100**) is actuated to immobilize a portion of the second instrument from the instrument immobilizer to the distal end of the second instrument at the target. In one example, the instrument immobilizer includes a retaining piece **1106** (FIG. **11**) that is actuated to engage the second instrument and immobilize it against the instrument immobilizer. At **2904**, the second instrument is uncoupled from the bracket. In one example, the bracket is uncoupled and removed from the second stage. The normalizing stage is removed from the instrument guide at **2906**. At **2908**, the saddle is uncoupled and removed from the instrument immobilizer. In another example, the normalizing stage is left coupled to the instrument guide and the saddle, and the saddle, instrument guide, and normalizing stage are uncoupled as a single unit from the instrument immobilizer. At **2910**, the non-immobilized portion of the second instrument is bent over and a cap is engaged to the instrument immobilizer to further retain the second instrument.

## CONCLUSION

The various embodiments of the normalizing stage in this document are presented as illustrative examples, and are not intended to be limiting. The normalizing stage embodiments discussed in this document will be capable of use with a variety of fixture assemblies, including the fixture assemblies discussed above. Additionally, the normalizing stage and the techniques discussed herein are not limited to advancing instruments toward, away or through target locations within a subject's brain. The normalizing stage apparatus and techniques are also applicable to targeting other locations within a subject. Furthermore, the normalizing stage and techniques discussed in this document may also be useful for moving instruments toward, away or through desired target locations within any material.

The normalizing stage described in this document provides a standard distance to a desired target. The standard distance provided with the first stage allows use of standard length, off the shelf, instruments, guide tubes, spacer tubes and obturators. The second stage moves correspondingly with the first stage. Therefore, positioning of the first stage a standard

distance from the desired target likewise positions the second stage with respect to the desired target area. Once the first stage is positioned the standard distance from the target, the second stage, moveably coupled to the first stage, moves the standard instrument toward, away and through the target location as desired. In other words, the first stage allows use of off the shelf instruments, tubes and the like, while the second stage moves the off the shelf instruments toward and/or away from the target. Thus the normalizing stage expedites the introduction of instruments to the target location. Additionally, the normalizing stage and the methods for using the same eliminate time-consuming calculations for physicians and/or technicians, for instance, calculations of the instrument, tube and obturator lengths. Moreover, the normalizing stage reduces errors by simplifying the introduction of instruments with standard length instruments, tubes and the like. Error is reduced by removing calculations of instrument lengths and the like from the procedure of use.

Moreover, the normalizing stage is a cost effective disposable unit that can be used for a procedure and disposed afterwards. The normalizing stage and other equipment described in this document are packaged sterile and used at the point of use. Sterile saline is readily available at most hospitals and clinics and is used prior to the procedure to fill the hydraulic examples described above.

It is to be understood that the above description is intended to be illustrative, and not restrictive. For example, the above described embodiments may be used in combination with each other. Many other embodiments will be apparent to those of skill in the art upon reading and understanding the above description. The scope of the invention should, therefore, be determined with reference to the appended claims, along with the full scope of equivalents to which such claims are entitled. In the appended claims, the terms "including" and "in which" are used as the plain-English equivalents of the respective terms "comprising" and "wherein." Moreover, in the following claims, the terms "first," "second," and "third," etc. are used merely as labels, and are not intended to impose numerical requirements on the objects.

What is claimed is:

1. An apparatus comprising:

a device for advancing a surgical instrument, the device including:

a base;

a first stage moveably coupled to the base;

a guide tube stop coupled with the first stage, wherein the guide tube stop includes at least one guide tube lumen, an outer ring having a notch, a rocker shaped to fit within the outer ring, the rocker including a stud, a seat received between an inner surface of the ring and the rocker, the seat having legs extending through the outer ring, and a thumbscrew passing through the notch and engaging the stud, the thumbscrew operable to move the rocker; and  
 a guide tube coupled with the guide tube stop, wherein the guide tube has an outer perimeter dimensioned and configured to snugly couple with a surface defining the guide tube lumen of the guide tube stop, and a guide tube flange adapted to engage with the guide tube stop.

2. The apparatus of claim 1, wherein the guide tube stop is sized and shaped to clamp and immobilize at least a portion of the guide tube.

3. The apparatus of claim 2, further comprising an obturator coupled with the guide tube, wherein the obturator has an outer perimeter dimensioned and configured to snugly couple with an inner perimeter of the guide tube, a blunt first end substantially coterminous with an end of the guide tube when

the obturator is positioned within the guide tube, and an obturator flange engageable with the guide tube.

4. The apparatus of claim 1, further comprising a spacer tube coupled with the guide tube, wherein the spacer tube has an outer perimeter dimensioned and configured to snugly couple with an inner perimeter of the guide tube, an inner perimeter dimensioned and configured to snugly couple with a first instrument to allow slidable movement therebetween and a spacer tube flange extending at least partially around a circumference of the spacer tube adapted to engage an upper surface of the guide tube.

5. The apparatus of claim 1, wherein the guide tube has an inner perimeter dimensioned and configured to snugly couple with a second instrument to allow slidable movement therebetween.

6. The apparatus of claim 1, further comprising a second stage and a rotatable threaded screw rotatably coupled to the first stage and the second stage, wherein the second stage is moveable relative to the first stage along the threaded screw.

7. An apparatus comprising:

a device for guiding a surgical instrument into a body of a patient, the device including:

a base including first and second guide rails extending from the base, wherein the base defines a trajectory for guiding the surgical instrument between the first and second guide rails;

a first stage moveably coupled to the base, wherein the first stage is moveable along the trajectory;

a second stage moveably coupled to the first stage, wherein the second stage is moveable relative to the first stage on or parallel to the trajectory and operable to move an instrument coupled thereto with respect to the base and the first stage, wherein at least the first stage is positionable at a first position where the first stage is at a desired distance from a target area in the body;

a guide tube stop received in a guide tube stop lumen defined in the first stage, wherein the guide tube stop includes at least one guide tube lumen;

a guide tube coupled with the guide tube stop, wherein the guide tube has an outer perimeter dimensioned and configured to snugly couple with the surface defining the guide tube stop lumen, and a flange extending at least partially around the outer perimeter of the guide tube, the flange adapted to engage an upper surface of the guide tube stop,

wherein the guide tube stop includes an outer ring having a notch, a rocker shaped to fit within the outer ring, the rocker including a stud, a seat received between an inner surface of the ring and the rocker, the seat having legs extending through the outer ring, and a thumbscrew passing through the notch and engaging the stud, the thumbscrew operable to move the rocker to clamp and immobilize the guide tube.

8. The apparatus of claim 7, further comprising a retaining assembly operable to immobilize at least a portion of the first instrument with respect to the second stage.

9. The apparatus of claim 7, further comprising a second stage actuator operable to advance the second stage and a portion of the instrument toward, away, and through the target area in the body.

10. The apparatus of claim 7, further comprising a rotatable threaded screw rotatably coupled to the first stage and the second stage, wherein the second stage is operable to advance with the first stage or separately advance along the rotatable screw toward and away from the body.

11. The apparatus of claim 7, wherein the guide tube stop includes a plurality of guide tube lumens disposed around a central lumen of the guide tube stop.

31

12. The apparatus of claim 7, further comprising an obturator coupled with the guide tube, wherein the obturator has an outer perimeter dimensioned and configured to snugly couple with the inner perimeter of the guide tube, a blunt first end substantially coterminous with an end of the guide tube when the obturator is positioned within the guide tube, and a flange extending at least partially around a circumference of the obturator and adapted to engage an upper surface of the guide tube.

13. The apparatus of claim 7, further comprising a spacer tube coupled with the guide tube, wherein the spacer tube has an outer perimeter dimensioned and configured to snugly couple with the inner perimeter of the guide tube, an inner perimeter dimensioned and configured to snugly couple with a first instrument to allow slidable movement therebetween and a flange extending at least partially around a circumference of the spacer tube adapted to engage an upper surface of the guide tube.

14. The apparatus of claim 7, wherein the guide tube has an inner perimeter dimensioned and configured to snugly couple with a second instrument to allow slidable movement therebetween.

15. The apparatus of claim 7, further comprising a measurement scale on the first stage and a reference marking on the second stage.

16. The apparatus of claim 7, further comprising a saddle aligned with the trajectory, wherein the saddle is rotatable about a first axis and arcuately positionable about a second axis substantially perpendicular to the first axis.

17. The apparatus of claim 7 further comprising an instrument guide coupled to the first stage, wherein the instrument guide defines at least one instrument guide lumen aligned with the trajectory.

18. The apparatus of claim 10, further comprising a first stage actuator threadably coupled to a stationary screw, wherein the stationary screw is positioned substantially parallel to the trajectory and coupled to the base, and the first stage actuator is rotatable for advancing the first stage along the trajectory and along the stationary screw.

19. The apparatus of claim 18, further comprising a circular fine measurement scale coupled to the rotatable screw and substantially perpendicular to the trajectory, and a reference marking on the first stage.

20. The apparatus of claim 14, further comprising a removable instrument bracket coupled with the second stage, wherein the instrument bracket is operable to immobilize at least a further portion of the second instrument with respect to the second stage at an offset position along the trajectory from the second stage and such that a distal end of the second instrument is substantially adjacent a prior location of a distal end of the first instrument.

21. The apparatus of claim 20, wherein the guide tube flange is moveable out of engagement with the guide tube stop along the trajectory to an intermediate position between the guide tube stop and the offset position to expose the second instrument at the end of the guide tube.

22. The apparatus of claim 21, further comprising an instrument immobilizer disposed along the trajectory, wherein the instrument immobilizer is operable to retain an exposed portion of the second instrument.

23. The apparatus of claim 15, wherein the measurement scale indicates a position of the instrument with respect to the target area in the body.

24. The apparatus of claim 15, wherein the measurement scale indicates a position of the instrument with respect to the target area in the body including an approach distance.

25. The apparatus of claim 24, wherein the approach distance is 15 millimeters.

32

26. The apparatus of claim 15, wherein the measurement scale indicates the position of the second stage relative to the first stage.

27. An apparatus comprising:

a device for advancing a surgical instrument into a body of a patient, the device including:

a base including first and second guide rails extending from the base, wherein the base defines a trajectory for guiding an instrument between the first and second guide rails;

a first stage moveably coupled to the base, wherein the first stage is moveable along the trajectory, the first stage including an upper portion defining first and second guide rail lumens slidably coupled with the first and second guide rails, and a lower portion defining two guide rail lumens slidably coupled with the first and second guide rails;

a first stage actuator having an inner surface threadably engaged with a stationary screw, the stationary screw substantially perpendicularly coupled to the base, the first stage actuator coupled to the lower portion of the first stage and rotatable to move the first stage along the trajectory and along the stationary screw;

a thumbscrew passing through the first stage and engageable with one of the first or second guide rails for immobilizing the first stage relative to the base;

a second stage moveably coupled to the first stage, wherein the second stage is moveable relative to the first stage on or parallel to the trajectory and operable to move an instrument coupled thereto with respect to the base and the first stage;

a rotatable threaded screw rotatably coupled to the first and second stages, the rotatable screw passing through the upper and lower portions of the first stage, the rotatable screw offset relative to the stationary screw; and

a second stage actuator cooperatively engaging the rotatable screw for advancing the second stage relative to the first stage;

wherein at least the first stage is in a first position where the first stage is a desired distance from a target area in the body.

28. The apparatus of claim 27, further comprising:

an instrument bracket removably coupled with the first stage, wherein the instrument bracket includes a distal collar base, a plurality of retaining prongs extending from the instrument bracket at a proximal end, and a thumbscrew, the instrument bracket operable to immobilize at least a portion of an instrument at a position along the trajectory and remote from the first stage.

29. The apparatus of claim 27, wherein the first guide rail has a substantially rectangular cross-section and the second guide rail has a substantially "T" cross-section.

30. The apparatus of claim 28, further comprising:

a measurement tube removably coupled to the instrument bracket, a proximal end of the measurement tube coupled against the retaining prongs, the measurement tube passing through a lumen of the distal collar base, wherein the measurement tube has a predetermined length for visual measurement of a corresponding instrument length.

31. The apparatus of claim 30, wherein the predetermined length of the measurement tube substantially corresponds to a distance from the instrument bracket to a desired target.

32. The apparatus of claim 30, wherein the measurement tube is substantially transparent.